

NEODENT®

PRODUCT CATALOGUE 2023

• ISSUE 01



years





Celebrating is a choice


Neodent® is celebrating its **30th** anniversary! Over time, millions of smiles have been created in partnership with professionals worldwide. Throughout the years, the Neodent® continues to celebrate the choice of creating new smiles every day, to change lives of patients in more than **80** countries where the brand is present.



Focused on ease of use, Neodent® Dental Implant Systems works on progressive treatment concepts such as immediacy with modern and reliable solutions to make implant dentistry possible. As the leader in immediate treatment, Neodent® has developed unique features taking into account the key biological principles designed to maximize predictability and achieve long-lasting results.

A photograph of a man and a woman smiling and laughing together in a garden. The man is on the left, wearing glasses and a light-colored polo shirt. The woman is on the right, wearing a light-colored top and a high-waisted skirt. The background is filled with green foliage.

Many reasons to celebrate



Impact on people's lives

From an idea to the reality of millions of smiles.



Technology and the future

From the possibility of restoration to immediate charging.
From traditional to digital flow.



Continuous improvement and innovation

From the first implant to GM and Zi.




Implantology 360 degrees

From conventional to digital and from laboratory to patient.



Expansion

From family business to multinational.
From Brazil to the world.



Connection with the sector
From 1 to 200 thousand dentists.



6th Neodent[®] Congress
The biggest event in Neodent[®] history where we will also celebrate the 30th anniversary.



ILAPEO
The partnership and cooperation between Neodent[®] and ILAPEO seeks to promote continuous education based on clinical and scientific evidence.



Neodent[®] GlobalPlay
Online and on demand content for your learning and improvement.



Solutions
Neodent[®] has proven product concepts and efficient treatment options, made by a dentist to dentists and focused on ease of use.

The choices we make
write our history



30 years of history that makes Neodent a company with a complete portfolio and the best innovative solutions for our costumers.

We built a legacy on quality and excellence, and today we are leading the way for the future of dentistry, being the most reliable and innovative partner for dentists all over the world.

The focus on our customers and the quality of our products is our passion, and with each passing year we expand our worldwide presence.

Our mission is to transform lives by creating new smiles every day.

Matthias Schupp • CEO of Neodent®



30 years of creating new smiles every day, an achievement that deserves a great celebration.

I am proud to see how much we have grown over time since our foundation, in 1993, until our first ceramic implant system, in 2022. I just see reasons to smile.

In 2015, with the full acquisition by Straumann Group, we started to spread our philosophy around the world and the gratitude to see Neodent present in over 80 countries with great results makes me happy and excited for the next years.

My commitment is that Neodent® keeps improving technology and solutions, with the purpose to enhance patients' life quality, in partnership with dedicated professionals, creating smiles every day.

I would like to thank everybody who was been part of our history until now and I invite you to celebrate with us the evolution of implantology, technology, the dentistry market, esthetics, patients, and Neodent®.

Dr. Geninho Thomé • Founder of Neodent®





Ceramic Implant System

Increasing expectations for esthetic treatments with shorter duration time, the Neodent® Ceramic Implant System combines the notions of flexibility, stability, and esthetic. This metal-free solution allows to immediately treat patients with high-end esthetic, thanks to the modern naturally tapered Ceramic implant design, with comprehensive ceramic prosthetic portfolio.

A new **mindset**

- A new flexibility mindset
- A new stability mindset
- A new esthetic mindset



DR GENINHO THOMÉ, from Brazil

“The patients are pursuing more and more esthetics results and we were able to come up with a product that is beautiful and also has injected ceramic technology, which makes it possible to make a high quality implant with an innovative, complex and metal-free technology.”





A new **flexibility mindset**

Looking to attend several demanding treatments, the Ceramic Implant System delivers the flexibility of a 2-pieces connection combined with a strong screw-retained ceramic-ceramic connection.



RELIABLE AND STRONG CERAMIC SYSTEM

The unique patented ZiLock® connection is designed with a longer screw which provides a secure engagement between the ceramic implant and the ceramic abutment. Additionally, it improves the ceramic performance by optimizing the force distribution along the internal connection.



FRIENDLY ZILOCK® CONNECTION

ZiLock® is a ceramic straight internal connection with 6 lobes and 6 points. This indexation results in a precise abutment positioning, protecting against rotation. The outcome is a user-friendly system that provides higher treatment flexibility when compared to one-piece implants.




A new **stability mindset**

Aiming to achieve stable immediate protocols, Zi combines a naturally tapered implant design and implant treated surface. Both designed to maximize stability and predictability in immediate treatments.

TAPERED DESIGN FOR PRIMARY STABILITY

Ceramic Implant System exhibits a modern tapered implant geometry designed for predictable immediacy in all bone types. This feature was designed to mimic the tapered shape of a natural tooth root, driving to achieve high primary stability.

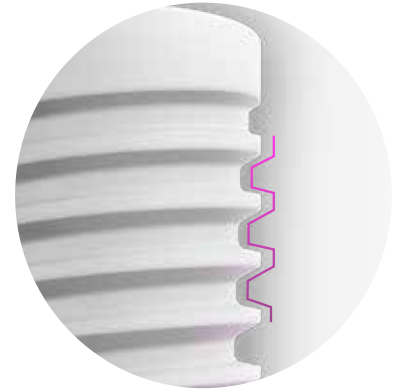


Double trapezoidal thread design.



Apically tapered with chamber flutes.

PREDICTABILITY WITH SAND-BLASTED AND ACID-ETCHED SURFACE

Zi features the sand-blasted and acid-etched surface treatment, presenting macro and micro roughness based on the highly successful Neoporos® treatment surface.

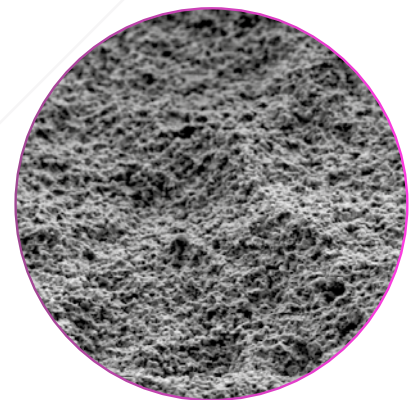

Representative image of the implant surface - Scanning Electron Microscope (SEM) magnification of 5000x.



DR FEDERICO MANDELLI, from Italy

“ Zi is a Ceramic Implant System that I can use with any immediate loading protocol. So I can keep my protocols the same, for titanium or ceramic, offering the same treatment for any case. ”



A new **esthetic mindset**

Seeking for an outstanding esthetic performance, Zi offers, from the material itself, Ceramic, to the comprehensive portfolio, a natural esthetic result.

OUTSTANDING ESTHETIC PERFORMANCE

Aiming to achieve superior esthetic results, Neodent® Ceramic Implant System seeks to offer outstanding natural performance, featuring a superior ceramic material, that supports a natural outcome of reconstruction due to its color that mimics natural teeth, and benefit from a high translucency compared to metals.

A PORTFOLIO TO ACHIEVE NATURAL ESTHETIC RESULTS

Ceramic prosthetic portfolio allows conventional or immediate protocol. In addition, preferable workflow can be applied from conventional to digital, providing a natural-looking restoration.



ZI BASE



Single-unit screw-retained prosthesis



Single-unit cement-retained prosthesis



Ø 3.75/4.5 mm



ZI BASE FOR C



Single-unit screw-retained prosthesis



Single-unit cement-retained prosthesis



Ø 4.65 mm



ZI CR ABUTMENT



Single-unit cement-retained prosthesis



Ø 4.0/4.5 mm

Neodent® Zi Implant Packaging

Neodent® packaging has been specially updated for easy handling and seeking to achieve a safe surgical procedure, providing practicality from implant stocking to the capture and transport and implant bed. The implant's features, such as type, diameter and length, are readily identifiable on the outside of the packaging.

Three self-adhesive labels are provided for recording in the patient's medical records and for reporting to the prosthesis team. They also allow traceability for all articles.



Package instruction of use



1. The cardboard and blister packagings must be opened, manually, without the use of sterile gloves. Break the seal of the cardboard packaging and remove the blister. Open the blister pack. Deposit the sterile flask over the surgical field.
NOTE: The clear tube and implant must be handled with a sterile surgical glove, in a surgical environment. Hold the bottle using the non-dominant hand and take the lid off.



2. The internal support containing the implant and transfer piece must come out attached to the lid. To do so, remove the lid and the clear tube's internal support in the axial direction without making any lateral movements.



3. Keep the support stable and remove the lid.



4. For installation, capture the implant transfer piece with the Hexagonal Connection, keeping it stable and slightly rotating the internal support, searching for the perfect fit between connection and transfer piece.





5. Take the transfer-implant assembly to the surgical cavity.

e-IFU – Electronic Instructions For Use

Neodent® innovates once more, providing an on-line platform designed to provide quick and practical use of its own products instructions: the e-IFU (Instructions For Use) website.

To facilitate access, have the article number, which can be found on the external packaging of the product, in this catalogue or with your local distributor. Once the article number is entered in the website, the professional will have access to relevant information to this product, such as description, indication for use, contraindications, handling, traceability and other features.

Access: ifu.neodent.com.br/en

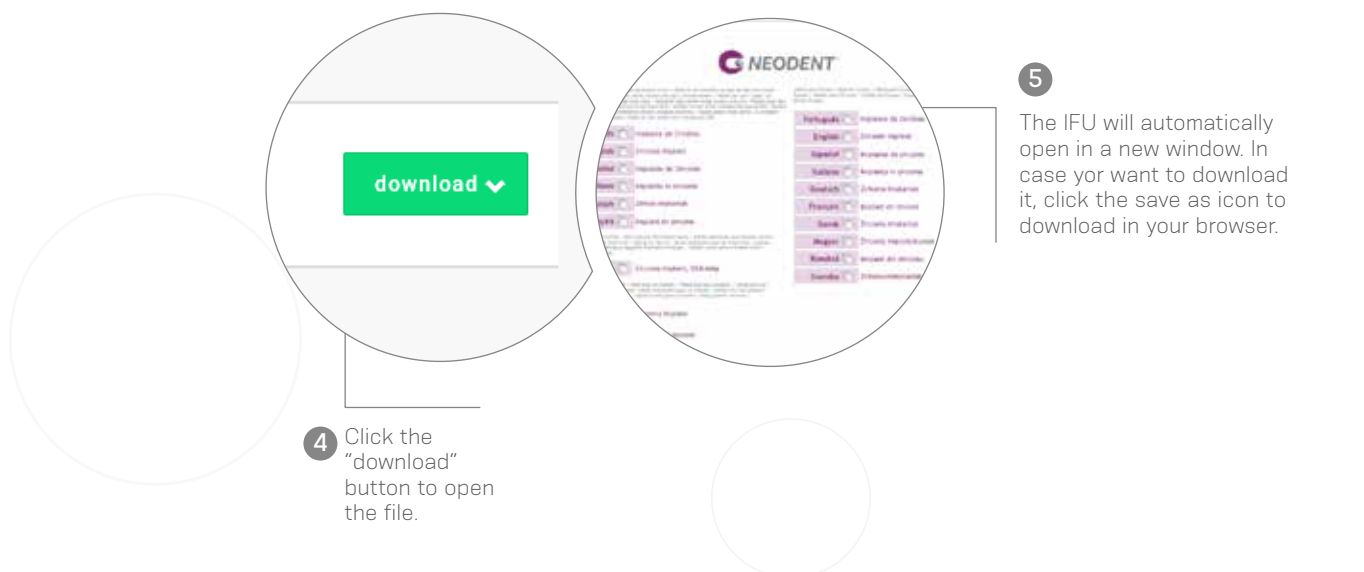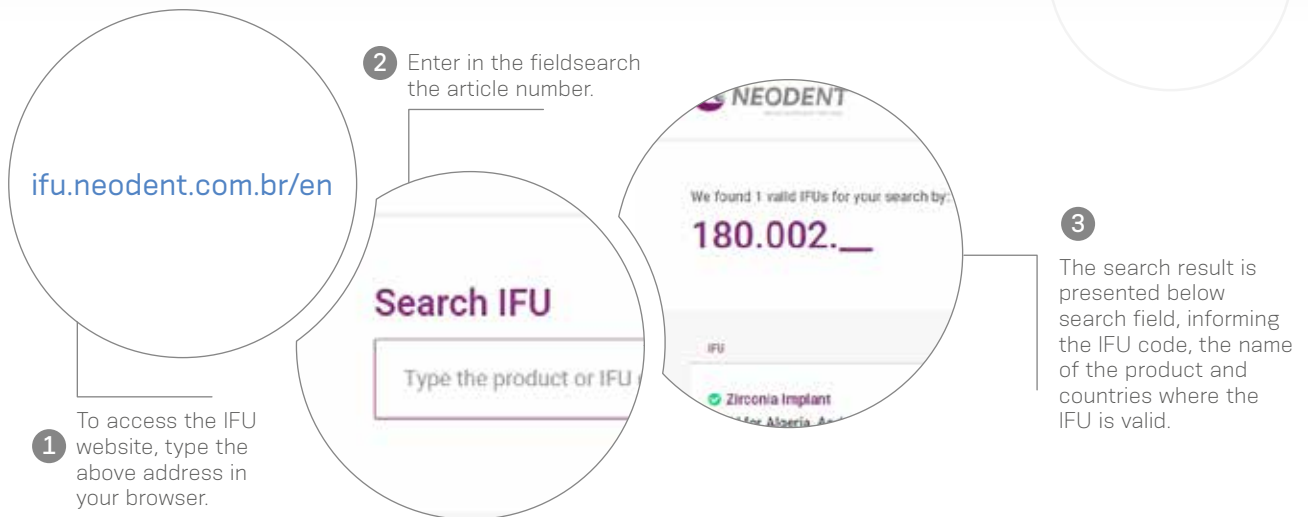

Zi Implant

PRODUCT FEATURES:

Implants Description:

- Naturally tapered design
- Compacting trapezoidal threads
- Double threaded implant
- Apically tapered with chamber flutes
- ZiLock® connection

Indications:

- Indicated for all types of bone density

Drilling features:


- Drilling speed: 800-1200 rpm for bone types I and II
- Drilling speed: 500-800 rpm for bone types III and IV.
- Countersink is required if used in bone types I, II and III with 300rpm.
- Bone tap is required if used in bone types I and II: contra angle: 30rpm/35 N.cm and torque wrench: maximum torque of 60N.cm
- Maximum insertion torque: 60 N.cm
- Minimum torque value for immediate loading: 35N.cm

Surface:


- Zi features the sand-blasted and acid-etched surface treatment, presenting macro and micro roughness based on the highly successful Neoporos® treatment surface.




Drill Sequence

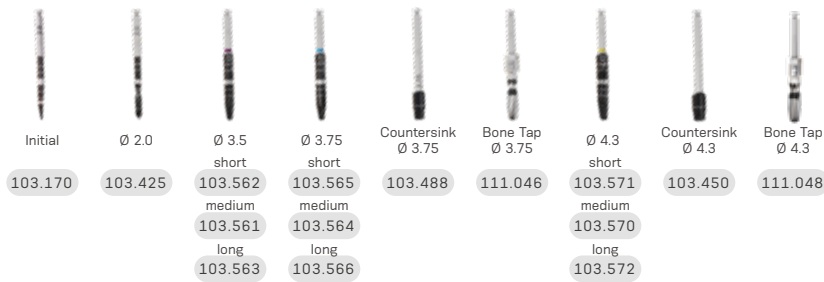


Ø 3.75 mm	✓*	✓	✓	✓	✓			
Ø 4.3 mm	✓*	✓	✓			✓	✓	✓

*Optional / Bone types I and II 

Ø 3.75 mm	✓*	✓	✓	✓	✓			
Ø 4.3 mm	✓*	✓	✓			✓	✓	

*Optional / Bone type III 

Ø 3.75 mm	✓*	✓	✓	✓				
Ø 4.3 mm	✓*	✓	✓			✓		

*Optional / Bone type IV 

Zi Implants



Zi Cover Screw



117.023

- :: Use the manual Neo Screwdriver (104.060);
- :: Do not exceed the insertion torque of 10 N.cm.

Zi Healing Abutments



Profile	1.5 mm	2.5 mm
Ø 3.75	106.233	106.234
Ø 4.5	106.235	106.236

- :: Use the manual Neo Screwdriver (104.060);
- :: Do not exceed the insertion torque of 10 N.cm.

Peek CR Abutment



Single-unit cement-retained temporary prosthesis




Ø 4.0/4.5 mm

- Neo screwdriver connection;
- Cementable area height: 5.0 mm;
- Gingival height: 1.5 & 2.5 mm;
- ZiLock® connection;
- Removable screw.



Installation Sequence

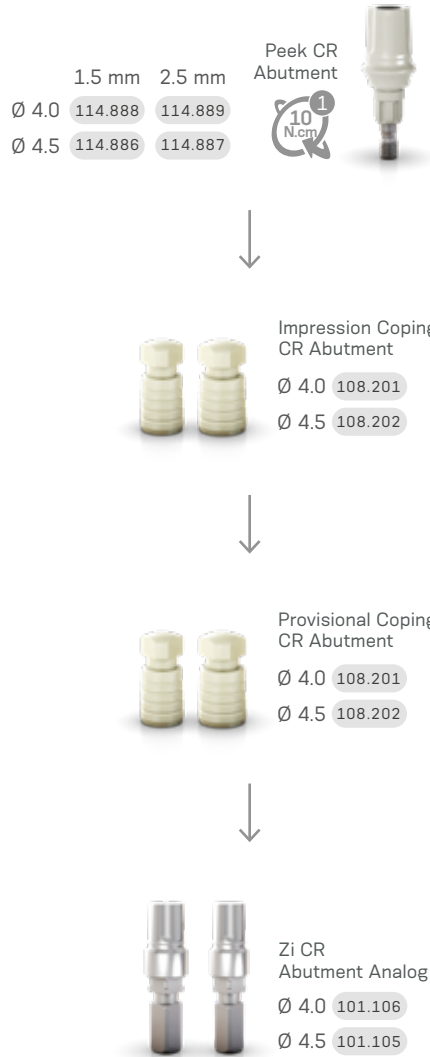

Hybrid use: can be used as an impression coping and a provisional abutment.

Drivers



Zi Base



Single-unit
screw-retained
prosthesis



Single-unit
cement-
retained
prosthesis



Ø 3.75/4.5 mm

Neo screwdriver connection;

Chimney height: 4.0 mm;

Gingiva height: 1.5 & 2.5 mm;

ZiLock® connection;

Removable screw.



Installation Sequence

Intraoral scanning



Zi
Implant
Scanbody
2
108.222



Hybrid Repositionable
Analog Zi Implant
(conventional/digital)
101.080



	1.5 mm	2.5 mm
Ø 3.75	135.254	135.255
Ø 4.5	135.256	135.257

Model Scanning



Zi Implant Exact
Impression Coping Open
and Closed Tray
2
Closed Open
Regular 108.186 108.188
Long 108.187 108.189



Hybrid Repositionable
Analog Zi Implant
(conventional/digital)
101.080



Zi
Implant
Scanbody
2
108.222



Zi Base
1
32 N.cm



Conventional



Zi Implant Exact
Impression Coping Open
and Closed Tray
2
Closed Open
Regular 108.186 108.188
Long 108.187 108.189



Hybrid Repositionable
Analog Zi Implant
(conventional/digital)
101.080



	1.5 mm	2.5 mm	Zi Base
Ø 3.75	135.254	135.255	1 32 N.cm
Ø 4.5	135.256	135.257	



Burn-out coping
Zi Base
Ø 3.75 118.343
Ø 4.5 118.325



Drivers

1



Neo
Screwdriver
Torque
Connection

+



Torque Wrench

2



Neo
Screwdriver
Torque
Connection

+



Manual
Screwdriver
Torque

Accessories



Abutment
replacement screw
116.289

Zi Base for C



Single-unit screw-retained prosthesis



Single-unit cement-retained prosthesis



Ø 4.65 mm

Design for CEREC® workflow;

Neo screwdriver connection;


Gingival height: 1.5 & 2.5 mm;

ZiLock® connection;

Removable screw.



Installation Sequence

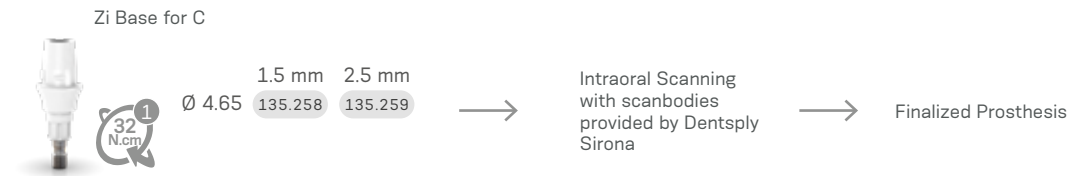

Workflow

Step 1

Gingiva height selection and ordering.



Select the Zi Base for C for C gingival height.



Order the Zi Base for C.

Please note that the scanbody has to be purchased directly from equipment manufacturer.

Step 2

Intra-oral scanning.



Insert the Zi Base for C in the Neodent® implant.



Insert scanbody on the Zi Base for C.

Step 3

Design and milling.



Select in the CAD software the comparable third-party Zi Base and perform the digital design.



Mill the digital design.

Step 4

Finalization and fixation.



- Check the fit of milled restoration in the patient's mouth and adapt it, if needed.
- Cement the restoration on the Zi Base for C and insert it into the patient's mouth.

CEREC digital library compatibility

Library	Sirona's Products				Compatible with implant System	
	Scanbody	REF Scanbody Omnicam	REF Scanbody Bluecam / Ineos	Griding block	Implant manufacturer	Implant system
NBB 3.4 L						
NB A 4.5 L						
SSO 3.5 L						
S BL 3.3 L	L	6431329	6431303	inCoris Zi meso L	Neodent®	GM, CM, HE, IIPlus
S BL 4.1 L						
BO 3.4 L						

Drivers

1

Neo Screwdriver Torque Connection

+



Torque Wrench

Accessories



Abutment replacement screw

116.289

Zi CR Abutment



Single-unit
cement-
retained
prosthesis




Ø 4.0/4.5 mm

- Neo screwdriver connection;
- Chimney height: 5.0 mm;
- Gingiva height: 1.5 & 2.5 mm;
- ZiLock® Connection;
- Removable screw.




Installation Sequence

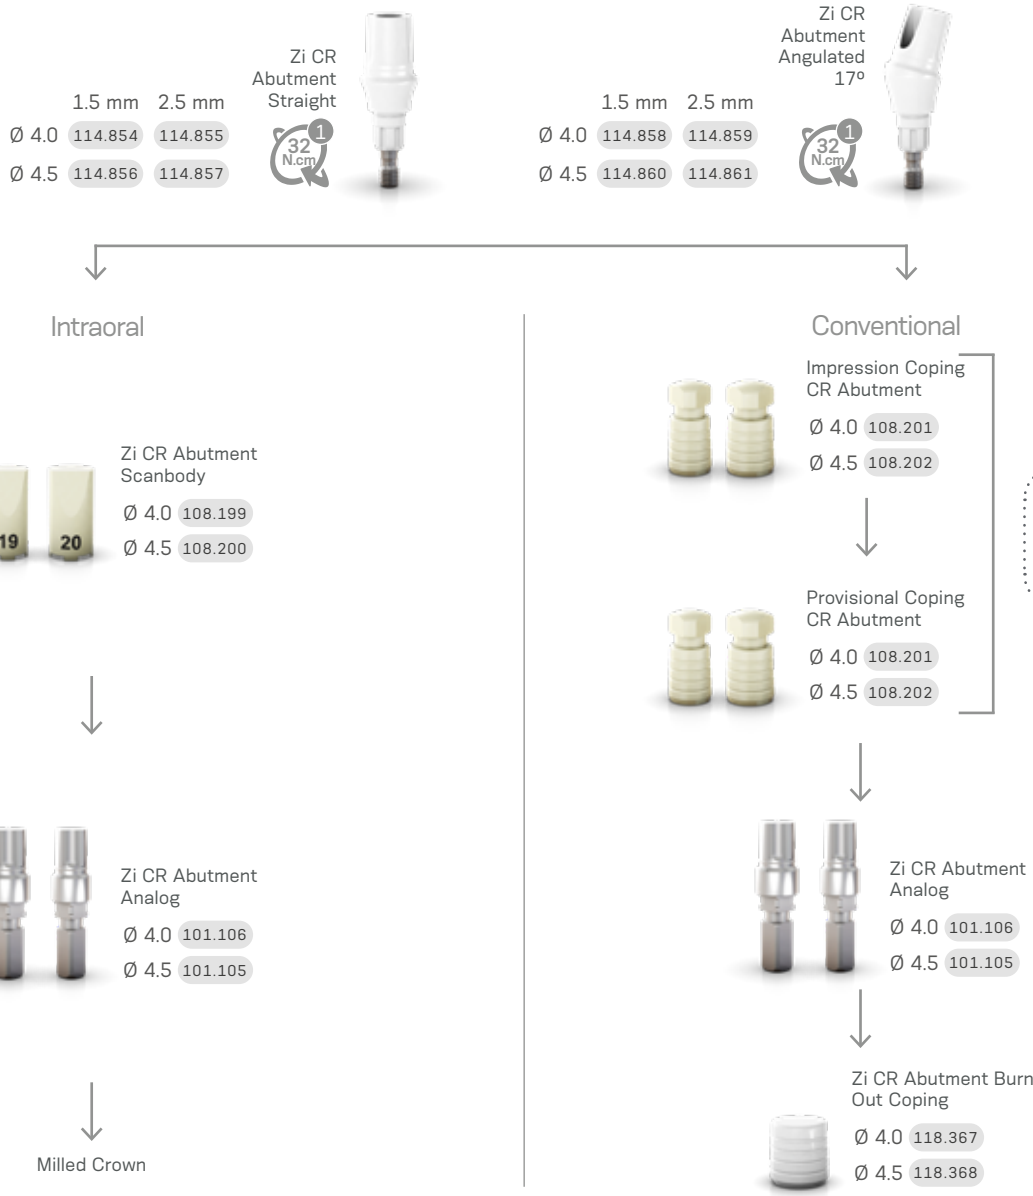

Drivers



Accessories



Zi Implant System Kit

Zi Compact Surgical Kit

Autoclavable polymer case.

The Kit allows the installation of Zi® Implants in all bone types.



Articles

- | | | | |
|---------|---|---------|---|
| 110.293 | Compact Surgical Kit Zirconia Implant | 103.426 | Drill extender |
| 103.488 | Countersink Drill For Zirconia Implant 3.75 | 104.060 | Neo Manual Screwdriver (medium) |
| 103.450 | Countersink Drill For Zirconia Implant 4.3 | 105.001 | Smart/ws Implant Driver - Torque Wrench (short) |
| 104.050 | Torque Wrench Driver | 105.002 | Smart/ws Implant Driver - Contra-angle |
| 111.046 | Bone Tap For Zirconia Implant 3.75 | 105.018 | Hex Connection - Torque Wrench (long) |
| 111.048 | Bone Tap For Zirconia Implant 4.3 | 105.132 | Neo Screwdriver Torque Connection |
| 103.170 | Initial drill Ø2.0 medium | 128.020 | Direction indicator Ø3.75 |
| 103.561 | Tapered Drill Ø3.5 | 128.022 | Direction indicator Ø4.3 |
| 103.564 | Tapered Drill Ø3.75 | 129.020 | Tapered X-ray Positioner 3.75 |
| 103.570 | Tapered Drill Ø4.3 | 129.013 | Tapered X-ray Positioner 4.3 |
| 103.492 | Tapered Drill Ø2.0 | 103.428 | Zi Bone Profile Drill With Guide |

Note: Items that compose Zi Neodent® Kit are sold separately.

Zi Implant System Instruments



Initial Drill

- :: Available in surgical steel;
- :: 2.0mm diameter.

103.170

Tapered Drills

- :: Available in surgical steel;
- :: Drill sequence for Zi Implants.

- 103.561 Tapered Drill Ø3.5
- 103.564 Tapered Drill Ø3.75
- 103.570 Tapered Drill Ø4.3
- 103.425 Tapered Drill Ø2.0
- 103.562 Tapered Drill (short) Ø3.5
- 103.563 Tapered Drill (long) Ø3.5
- 103.565 Tapered Drill (short) Ø3.75
- 103.566 Tapered Drill (long) Ø3.75
- 103.571 Tapered Drill (short) Ø4.3
- 103.572 Tapered Drill (Long) Ø4.3
- 103.574 Tapered Drill (short) Ø5.0
- 103.575 Tapered Drill (Long) Ø5.0



Countersink Drills

- :: Available in surgical steel;

- 103.488 Ø3.75
- 103.450 Ø4.3



Bone Tap

- :: Available in surgical steel;

- 111.046 Ø3.75
- 111.048 Ø4.3



Torque Wrench

- :: Available in surgical steel;
- :: Fitting for square connections;
- :: Collapsible Wrench that allows for proper assembly cleaning.

104.050



Neo Screwdriver Torque Connection - Torque Wrench

- :: Available in surgical steel;
- :: Yellow color for line identification.

- | Short | Medium | Long |
|---------|---------|---------|
| 16.5 mm | 22 mm | 32 mm |
| 105.133 | 105.132 | 105.157 |



Neo Manual Screwdriver


- :: Available in surgical steel;
- :: Yellow color for line identification

- | Short | Medium | Long |
|---------|---------|---------|
| 21 mm | 25 mm | 37 mm |
| 104.058 | 104.060 | 104.070 |



Direction Indicators

- :: Available in titanium;
- :: Instrument to guide the implant position;
- :: Diameter of central band corresponds to GM and Zi Implant diameter;
- :: Smaller side to be used after Ø2.0mm drill;
- :: Larger side to be used after the last drill before implant installation.



- 3.0/3.75 128.020
- 3.6/4.3 128.022

Drill Extension

- :: Available in surgical steel;
- :: Fit the drill directly into the Drill Extension.

103.426



Zi Bone Profile Drill with Guide

- :: Available in surgical steel;
- :: Used in the surgical second step;
- :: Conforms the bone around the implant platform, preparing the emergence profile to be suitable to prosthetic components.

103.428



Tapered X-Ray Positioner

- :: Check the axis in relation to adjacent roots using numbers identification.

- | | |
|---------|---------|
| Ø3.75 | Ø4.3 |
| 129.020 | 129.013 |



Grand Morse®

GREATNESS IS AN ACHIEVEMENT



GRAND RELIABILITY

STABLE AND STRONG FOUNDATION
DESIGNED FOR LONG TERM SUCCESS


The implant-abutment interface is crucial for a successful long term functional and esthetic result. The Neodent® Grand Morse® connection offers a unique combination based on proven concepts: a platform switching associated with a deep 16° Morse Taper including an internal indexation for a strong and stable connection designed to achieve long-lasting results.

24



1 Platform Switching

Abutment design with a narrower diameter than the implant coronal area, enabling the platform switching concept⁽⁵⁻⁹⁾.



2 Internal Indexation

Precise abutment positioning, protection against rotation and easy handling.




3 Deep Connection

Allowing a large contact area between the abutment and the implant for an optimal load distribution.



4 16° Morse Taper Connection

Designed to ensure tight fit for an optimal connection sealing.



DR JOE BHAT, from United Kingdom

"The new GM line has been the most effective tool that I have used in my practice. With regard to full-arch reconstruction and for immediate loading. "





GRAND SIMPLICITY

EASE OF USE AT ITS BEST

Implant therapy has become an integral part of clinical dentistry, with ever increasing numbers of patients seeking such treatment. The Neodent® Grand Morse® Implant System is smartly engineered providing efficiency and simplicity within the dental treatment network for both surgical to restoratives steps.

ONE PROSTHETIC PLATFORM

All Neodent® Grand Morse® implants feature the unique Grand Morse® connection regardless of the implant diameter.



ONE SCREWDRIVER

The Neo Screwdriver has a star attachment offering reliability and durability compatible with all Neodent® Grand Morse® healing abutments and cover screws and most of the restorative screws.



ONE IMPLANT DRIVER

The Neodent® implant driver allows an easy and reliable implant pick up and placement.



ONE SURGICAL KIT

Intuitive and functional compact surgical kit, that allows the place of Helix GM® implants in all bone types.



DR MICHELE ANTONIO LOPEZ, from Italy

“ Helix GM Implant give me many solutions, because it’s a very easy implant system, one only platform, an universal implant very stable and full of solutions from a prosthetic point of view. ”



GRAND STABILITY

STABLE AND STRONG FOUNDATION DESIGNED FOR LONG TERM SUCCESS

The increasing expectations for shortened treatment duration represent a significant challenge for dental professionals. The Neodent® Grand Morse® system offers a unique implant design featuring the innovative Acqua hydrophilic surface designed to maximize primary stability and predictability in immediate protocols.



HELIX® - OPTIMAL IMPLANT DESIGNED TO ACHIEVE HIGH PRIMARY STABILITY

Helix® Grand Morse® is an innovative hybrid implant design maximizing treatment options and efficiency in all bone types.

Fully tapered body design

- Coronal: 2° - 12°
- Apex: 16°
- » Allowing under-osteotomy




Hybrid contour

- Coronal: Cylindrical
- Apex: Conical
- » For stability with vertical placement flexibility



Active apex

- Soft rounded small tip
- Helical flutes
- » Enabling immediate loading



Dynamic progressive thread design

- Coronal: Trapezoidal > compressing
- Apex: V-Shape > Self-tapping
- » Achieving high primary stability in all bone types



Acqua hydrophilic surface

Designed for high treatment predictability

acqua



Titamax®

Vertical placement flexibility.
Bone types I & II.



Drive®

High primary stability in
challenging bone types.
Bone types III & IV.



GRAND ESTHETICS

DELIVER IMMEDIATE
NATURAL ESTHETICS



DR PAULO CARVALHO, from Portugal

“On the prosthetic part, the emergence profiles of the abutments, and everything that happens from the connection above, works and makes success in the long term. //”

Nowadays, patients expect both short treatment times and esthetic results. The Neodent® Grand Morse® restorative portfolio offers flexibility to simplify soft tissue management respecting the biological distances for achieving immediate function and esthetics.



Titanium Temporary Abutment



Pro-Peek Abutment



Titanium Base



Titanium Base C



Titanium Base for Bridge



Titanium Block (AG or Medentika Holder)



CoCr Abutment



Anatomic Abutment (straight and angled)



Universal Abutment (straight and angled)



Abutment



Angled Mini Conical Abutment



Novaloc (straight and angled)



Titanium Base AS



Straight Mini Conical Abutment




Micro Abutment



Single-unit screw-retained prosthesis




Single-unit cement-retained prosthesis




Overdenture



Multiple-unit screw-retained prosthesis



Multiple-unit cement-retained prosthesis



Temporary

Neodent® Grand Morse Implant Packaging

Neodent® implant packaging has been updated to a concept that provides convenience and safety through all steps of the procedure, from storage to the placement of the implant. The new packaging aids in identification of both the implant model as well as its diameter and length, regardless of its storage position.



Package instruction of use



1. After breaking the sterility seal on the blister, hold the primary package (vial) and twist the lid to open it.



2. To remove the implant from the vial lift the cap up, which has the stand and implant attached to it.




3. To secure the implant, grip both sides of the implant carrier.



4. While gripping the implant carrier, remove the lid.



5. To capture the implant with the contra-angle handpiece attachment, grip the implant carrier while placing the attachment into the implant chamber.

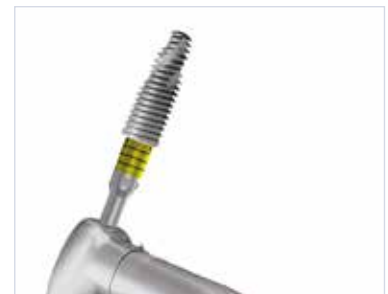

6. The implant can now be transported to the surgical site.

e-IFU – Electronic Instructions For Use

Neodent® innovates once more, providing an on-line platform designed to provide quick and practical use of its own products instructions: the e-IFU (Instructions For Use) website.

To facilitate access, have the article number, which can be found on the external packaging of the product, in this catalogue or with your local distributor. Once the article number is entered in the website, the professional will have access to relevant information to this product, such as description, indication for use, contraindications, handling, traceability and other features.

Access: ifu.neodent.com.br/en



ifu.neodent.com.br/en

- 1 To access the IFU website, type the above address in your browser.

- 2 Enter in the field search the article number.

Search IFU

Type the product or IFU

NEODENT

We found 4 valid IFUs for your search by:
140.985.____

We
GM Hells Implant
Valid for Argentina, Bolivia, Bosnia-Herzegovina, Dominican Rep., Egypt, Hong Kong, Mexico, Montenegro, Morocco, Vietnam

- 3 The search result is presented below search field, informing the IFU code, the name of the product and countries where the IFU is valid.

download ▼

- 4 Click the "download" button to open the file.

NEODENT



- 5 The IFU will automatically open in a new window. In case you want to download it, click the save as icon to download in your browser.



NeoPoros

Constant evolution and safety guarantee.

Based on the abrasive sandblasting concept followed by acid etching, the **NeoPoros** surface promotes, by using controlled grain oxides, cavities on the implant surface that then are uniformed with the acid etching technique.

The whole process of obtaining this surface is guaranteed due to automated time, speed, pressure and particle size control.

Several scientific studies continue to be performed so that the **NeoPoros** surface may be always evolving and promoting much more reliability for you.

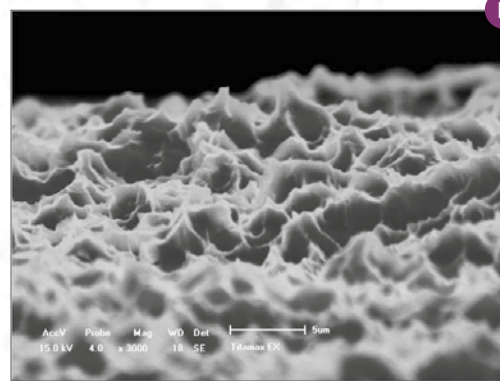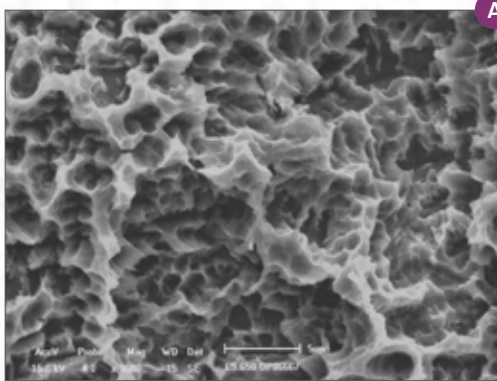

Controlled roughness on all implant surface. Scanning electron microscopy (A) shows macro (15-30µm) and (B) microtopography (0,3 - 1,3µm).

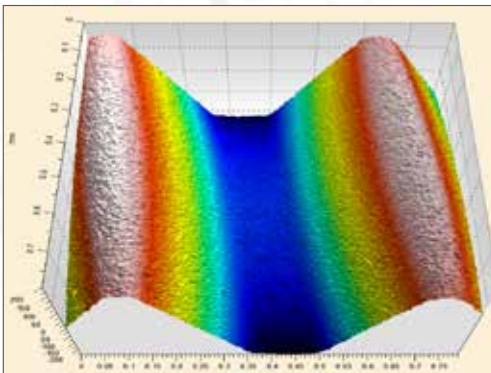


Image taken by confocal microscopy.
Roughness and Microtopography.
($S_a = 0,3 - 1,3 \mu\text{m}$; $S_z = 6,0 - 15,5 \mu\text{m}$).



DR ANA TADORIC, from Serbia

“I like the immediacy and I like the immediate loading. That is something that our patients are demanding in everyday practice more and more. So this is perfect for me.”

acqua®

Acqua Hydrophilic Surface designed for high treatment predictability.

The Neodent® Acqua hydrophilic surface is the next level of the highly successful S.L.A. type of surface developed to achieve successful outcomes even in challenging situations, such as soft bone or immediate protocols.^[1-4]

Hydrophilicity

The hydrophilic surface presents a smaller contact angle when in contact with hydrophilic liquids. This provides greater accessibility of organic fluids to Acqua implant surface.^[2]

Surface comparison

Lab generated images.



NeoPoros surface.



*Acqua Hydrophilic
Surface.*



DR GERT SAUER, from South Africa

“ The design of Neodent® GM Helix Acqua allows for immediate loading for all cases with predictable results. That is the main reason why I’m using Neodent®; even in cases with poor bone quality we can achieve primary stability. This results in predictable solutions for all of our patients. ”

Neodent easypack

GROW WITH PEACE OF MIND

Neodent® has developed EasyPack to simplify your daily practice. An all-in-one set that offers everything you need to grow while performing dental implant therapy with confidence, convenience and guidance.



GROW WITH CONFIDENCE

Choose a brand and products you can rely on



GROW WITH CONVENIENCE

The certainty of having everything in one package





GROW WITH GUIDANCE

All workflows in simple steps



THE NEODENT® EASYPACK INCLUDES

- 1 Grand Morse® Helix Implant
- 2 Grand Morse® Cover Screw
- 3 Grand Morse® Healing Abutment
- 4 Grand Morse® Hybrid Implant Analog
- 5 Grand Morse® 3-in-1 Neodent® Smart Abutment™ **NEW**

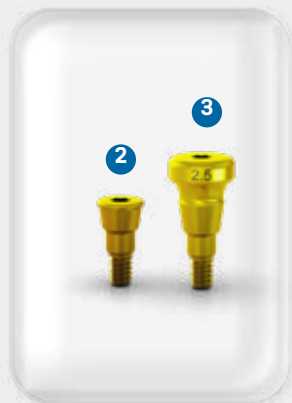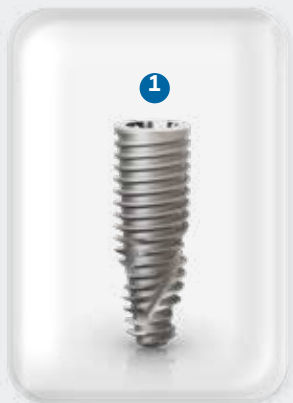



CONVENTIONAL
WORKFLOW




DIGITAL
WORKFLOW

Reliable guided workflow with the 3-in-1 GM Smart Abutment





The combination of the GM Smart Abutment, a unique patented solution combining a closed tray impression coping, a digital scanbody and a temporary abutment in a single piece, with healing components and the analog allows you to choose a restorative path guided for achieving predictable results.

IMPLANT PLACEMENT HEALING PHASE IMPRESSION PHASE TEMPORARY RESTORATION FINAL RESTORATION

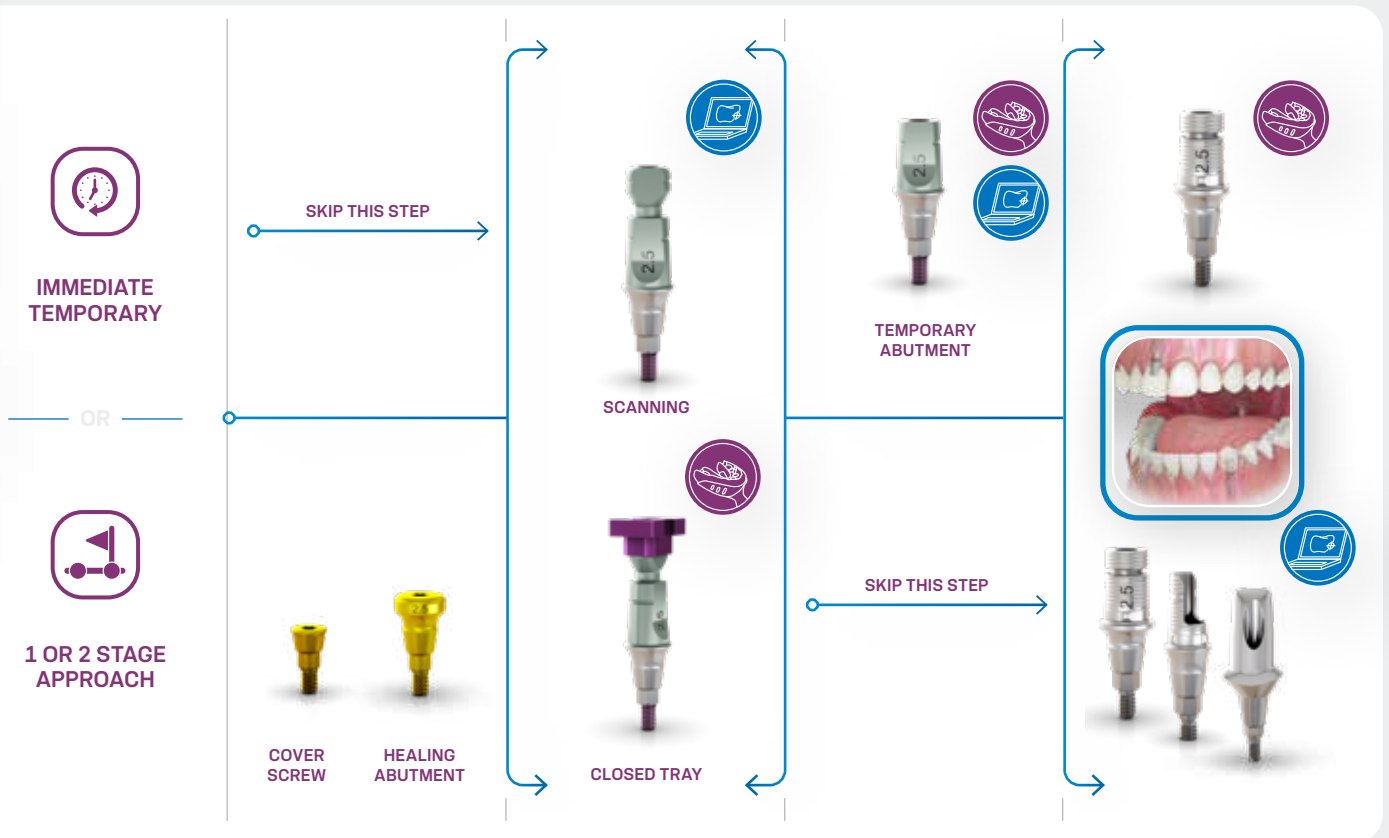

NEODENT® EASYPACK PRODUCT OPTIONS

	Ø 3.5		Ø 3.75		Ø 4.0		Ø 4.3		Ø 5.0	
	Acqua	NeoPoros	Acqua	NeoPoros	Acqua	NeoPoros	Acqua	NeoPoros	Acqua	NeoPoros
8.0	138.089	138.005	138.113	138.029	138.137	138.053	138.158	138.074	138.182	138.170
10.0	138.095	138.011	138.119	138.035	138.143	138.059	138.161	138.077	138.185	138.173
11.5	138.101	138.017	138.125	138.041	138.149	138.065	138.164	138.080	138.188	138.176
13.0	138.107	138.023	138.131	138.047	138.155	138.071	138.167	138.083	138.191	138.179

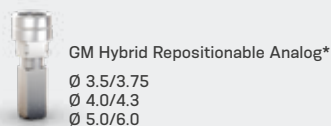

*according to implant diameter

Helix GM[®]

PRODUCT FEATURES:

Implants Description:

- Full dual tapered implant;
- Hybrid contour with a cylindrical coronal part and conical on the apical area;
- Active apex including a soft rounded small tip and helicoidal flutes;
- Dynamic progressive thread design: from compressing trapezoidal threads on the coronal area to self-tapping V-shape threads on the apical part;
- Double threaded implant;
- Grand Morse[®] connection.

Indications:

- Indicated for all types of bone density and implant immediate placement post extraction.

Drilling features:

- Contour drill is required in bone types I and II;
- Final pilot drills are highly recommended in bone types I and II;
- Implant should be positioned 1 or 2 mm below bone level;
- Drilling speed: 800-1200 rpm for bone type I and II;
- Drilling speed: 500-800 rpm for bone type III and IV;
- Implant insertion speed: 30 rpm;
- Maximum torque for implant placement: 60 N.cm.




Available with:


NeoPoros or 

Drill Sequence

	Initial 103.170	Ø 2.0 103.425	Ø 3.5 103.561	Ø 3.5+ 103.578	Ø 3.5 103.513	Ø 3.75 103.564	Ø 3.75+ 103.579	Ø 3.75 103.514	Ø 4.0 103.567	Ø 4.0+ 103.580	Ø 4.0 103.515	Ø 4.3 103.570	Ø 4.3+ 103.581	Ø 4.3 103.516	Ø 5.0 103.573	Ø 5.0+ 103.582	Ø 5.0 103.517	Ø 6.0 103.576	Ø 7.0 103.577
Ø 3.5	✓*	✓	✓	✓	✓														
Ø 3.75	✓*	✓	✓				✓	✓											
Ø 4.0	✓*	✓	✓			✓			✓	✓									
Ø 4.3	✓*	✓	✓			✓			✓			✓	✓	✓					
Ø 5.0	✓*	✓	✓			✓			✓			✓			✓	✓			


*Optional / Bone types I and II 

Ø 3.5	✓*	✓	✓																
Ø 3.75	✓*	✓	✓			✓*													
Ø 4.0	✓*	✓	✓					✓*											
Ø 4.3	✓*	✓	✓			✓						✓*							
Ø 5.0	✓*	✓	✓			✓						✓			✓*				
Ø 6.0	✓*	✓	✓			✓						✓			✓			✓	
Ø 7.0	✓*	✓	✓			✓						✓			✓			✓	✓*


*Optional / Bone types III and IV 

Drill Sequence with Neodent® Control System

	Initial 103.170	Ø 2.0 103.492	Ø 3.5 103.493	Ø 3.5+ 103.500	Ø 3.5 103.513	Ø 3.75 103.494	Ø 3.75+ 103.501	Ø 3.75 103.514	Ø 4.0 103.495	Ø 4.0+ 103.502	Ø 4.0 103.515	Ø 4.3 103.496	Ø 4.3+ 103.503	Ø 4.3 103.516	Ø 5.0 103.497	Ø 5.0+ 103.504	Ø 5.0 103.517	Ø 6.0 103.498	Ø 7.0 103.499
Ø 3.5	✓*	✓	✓	✓	✓														
Ø 3.75	✓*	✓	✓				✓	✓											
Ø 4.0	✓*	✓	✓			✓			✓	✓									
Ø 4.3	✓*	✓	✓			✓			✓			✓	✓	✓					
Ø 5.0	✓*	✓	✓			✓			✓			✓			✓	✓			

*Optional / Bone types I and II 

Ø 3.5	✓*	✓	✓																
Ø 3.75	✓*	✓	✓			✓*													
Ø 4.0	✓*	✓	✓					✓*											
Ø 4.3	✓*	✓	✓			✓						✓*							
Ø 5.0	✓*	✓	✓			✓						✓			✓*				
Ø 6.0	✓*	✓	✓			✓						✓			✓			✓	
Ø 7.0	✓*	✓	✓			✓						✓			✓			✓	✓*

*Optional / Bone types III and IV 

Helix GM® Implants

Ø 3.5	Acqua	NeoPoros	Ø 3.75	Acqua	NeoPoros	Ø 4.0	Acqua	NeoPoros	Ø 4.3	Acqua	NeoPoros
8.0	140.943	109.943	8.0	140.976	109.976	8.0	140.982	109.982	8.0	140.948	109.948
10.0	140.944	109.944	10.0	140.977	109.977	10.0	140.983	109.983	10.0	140.949	109.949
11.5	140.945	109.945	11.5	140.978	109.978	11.5	140.984	109.984	11.5	140.950	109.950
13.0	140.946	109.946	13.0	140.979	109.979	13.0	140.985	109.985	13.0	140.951	109.951
16.0	140.947	109.947	16.0	140.980	109.980	16.0	140.986	109.986	16.0	140.952	109.952
18.0	140.988	109.988	18.0	140.981	109.981	18.0	140.987	109.987	18.0	140.989	109.989

Ø 5.0	Acqua	NeoPoros	Ø 6.0	Acqua	NeoPoros	Ø 7.0	Acqua	NeoPoros
8.0	140.953	109.953	8.0	140.1009	109.1009	8.0	140.1059	109.1059
10.0	140.954	109.954	10.0	140.1010	109.1010	10.0	140.1060	109.1060
11.5	140.955	109.955	11.5	140.1011	109.1011	11.5	140.1061	109.1061
13.0	140.956	109.956	13.0	140.1012	109.1012	13.0	140.1062	109.1062
16.0	140.957	109.957						
18.0	140.990	109.990						

GM Cover Screw	0 mm	2 mm
	117.021	117.022

:: Use the manual Neo Screwdriver (104.060);
 :: Do not exceed the insertion torque of 10 N.cm.

GM Healing Abutment

	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm
Ø 3.3	106.207	106.208	106.209	106.210	106.211	106.212
Ø 4.5	106.213	106.214	106.215	106.216	106.217	106.218
Ø 5.5		106.250	106.251	106.252	106.253	
Ø 6.5		106.254	106.255	106.256	106.257	

:: Use the manual Neo Screwdriver (104.060);
 :: Do not exceed the insertion torque of 10 N.cm.

GM Customizable Healing Abutment

	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm	6.5 mm
Ø 5.5	106.223	106.224	106.225	106.226	106.227	
Ø 7.0		106.228	106.229	106.230	106.231	106.232

:: Use the manual Neo Screwdriver (104.060);
 :: Do not exceed the insertion torque of 10 N.cm.

Drive GM[®]

PRODUCT FEATURES:

Implants Description:

- Tapered implant;
- Square shape threads;
- Double threaded implant;
- Reverse cutting chambers distributed across the implant body;
- Rounded apex with a sharp edge;
- Grand Morse[®] connection.

Indications:

- Indicated for bone types III and IV and implant immediate placement post-extraction;

Drilling features:

- Final pilot drill is optional in bone types III and IV;
- Implant should be positioned 1 or 2 mm below bone level;
- Drilling speed: 500-800 rpm;
- Implant insertion speed: 30 rpm;
- Maximum torque for implant placement: 60 N.cm.





















Drill Sequence

								
	Initial	Ø 2.0	Ø 3.5	Ø 3.5	Ø 4.3	Ø 4.3	Ø 5.0	Ø 5.0
	103.170	103.425	103.561	103.513	103.570	103.516	103.573	103.517
Ø 3.5 mm	✓	✓	✓	✓ *				
Ø 4.3 mm	✓	✓	✓		✓	✓ *		
Ø 5.0 mm	✓	✓	✓		✓		✓	✓ *

*Optional / Bone types III and IV



Drive GM® Implants

		8.0 mm	10.0 mm	11.5 mm	13.0 mm	16.0 mm	18.0 mm
Ø 3.5							
	Acqua	140.958	140.959	140.960	140.961	140.962	140.963
	NeoPoros	109.958	109.959	109.960	109.961	109.962	109.963
Ø 4.3							
	Acqua	140.964	140.965	140.966	140.967	140.968	140.969
	NeoPoros	109.964	109.965	109.966	109.967	109.968	109.969
Ø 5.0							
	Acqua	140.970	140.971	140.972	140.973	140.974	140.975
	NeoPoros	109.970	109.971	109.972	109.973	109.974	109.975

GM Cover Screw



0 mm	2 mm
117.021	117.022

:: Use the manual Neo Screwdriver (104.060);
 :: Do not exceed the insertion torque of 10 N.cm.

GM Healing Abutment



	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm
Ø 3.3	106.207	106.208	106.209	106.210	106.211	106.212
Ø 4.5	106.213	106.214	106.215	106.216	106.217	106.218
Ø 5.5		106.250	106.251	106.252	106.253	
Ø 6.5		106.254	106.255	106.256	106.257	

:: Use the manual Neo Screwdriver (104.060); :: Do not exceed the insertion torque of 10 N.cm.

GM Customizable Healing Abutments



Profile	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm	6.5 mm
Ø 5.5	106.223	106.224	106.225	106.226	106.227	
Ø 7.0		106.228	106.229	106.230	106.231	106.232

Titamax GM[®]

PRODUCT FEATURES:

Implants Description:

- Cylindrical implant (parallel walls);
- V-shape threads;
- Double threaded implant;
- Self tapping apex;
- Grand Morse[®] connection.

Indications:

- Indicated for bone types I and II or grafted areas such as bone block.

Drilling features:

- Final pilot drill is highly recommended in bone types I and II;
- Implant should be positioned 1 or 2 mm below bone level;
- Self tapping implant which doesn't require the use of bone tap or contour drill;
- Drilling speed: 800-1200 rpm;
- Implant insertion speed: 30 rpm;
- Maximum torque for implant placement: 60 N.cm.




Available with:

NeoPoros[®] or

acqua[®]

Drill Sequence

	Initial	Ø 2.0	Ø 2/3	Ø 2.8	Ø 3.0	Ø 3.5	Ø 3.3	Ø 3.75	Ø 4.0	Ø 3.8	Ø 4.3	Ø 5.0
	103.170	103.162	103.213	103.163	103.164	103.513	103.166	103.514	103.515	103.167	103.168	103.517
Ø 3.5 mm	✓	✓		✓		✗						
Ø 3.75 mm	✓	✓	✓		✓			✓				
Ø 4.0 mm	✓	✓	✓		✓		✓		✓			
Ø 5.0 mm	✓	✓	✓		✓			✓		✓	✓	✓

Bone types I and II 

Titamax GM® Implants

		7.0 mm	8.0 mm	9.0 mm	11.0 mm	13.0 mm	15.0 mm	17.0 mm
Ø 3.5	Acqua	140.906	140.907	140.908	140.909	140.910	140.911	140.912
	NeoPoros	109.906	109.907	109.908	109.909	109.910	109.911	109.912
Ø 3.75	Acqua	140.899	140.900	140.901	140.902	140.903	140.904	140.905
	NeoPoros	109.899	109.900	109.901	109.902	109.903	109.904	109.905
Ø 4.0	Acqua	140.913	140.914	140.915	140.916	140.917	140.918	140.919
	NeoPoros	109.913	109.914	109.915	109.916	109.917	109.918	109.919
Ø 5.0	Acqua	140.920	140.921	140.922	140.923	140.924		
	NeoPoros	109.920	109.921	109.922	109.923	109.924		

GM Cover Screw



	0 mm	2 mm
	117.021	117.022

:: Use the manual Neo Screwdriver (104.060);
 :: Do not exceed the insertion torque of 10 N.cm.

GM Healing Abutment



	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm
Ø 3.3	106.207	106.208	106.209	106.210	106.211	106.212
Ø 4.5	106.213	106.214	106.215	106.216	106.217	106.218
Ø 5.5		106.250	106.251	106.252	106.253	
Ø 6.5		106.254	106.255	106.256	106.257	

:: Use the manual Neo Screwdriver (104.060); :: Do not exceed the insertion torque of 10 N.cm.

GM Customizable Healing Abutments



Profile	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm	6.5 mm
Ø 5.5	106.223	106.224	106.225	106.226	106.227	
Ø 7.0		106.228	106.229	106.230	106.231	106.232

GM Abutment



Single-unit screw-retained prosthesis



Ø 4.8 mm

Recommended for posterior region.

Consider in addition 1.5 - 2.0 mm for the restorative material;
 Minimum interocclusal space of 4.9 mm from the mucosa level;
 With internal threads for a secure engagement of the screw;
 Exact;
 Neo Removable Screw;



Installation Sequence


0.8 mm 1.5 mm 2.5 mm GM Exact Abutment with Neo Removable Screw
 115.269 115.270 115.271
 3.5 mm 4.5 mm
 115.272 115.273



Intraoral



Model Scanning

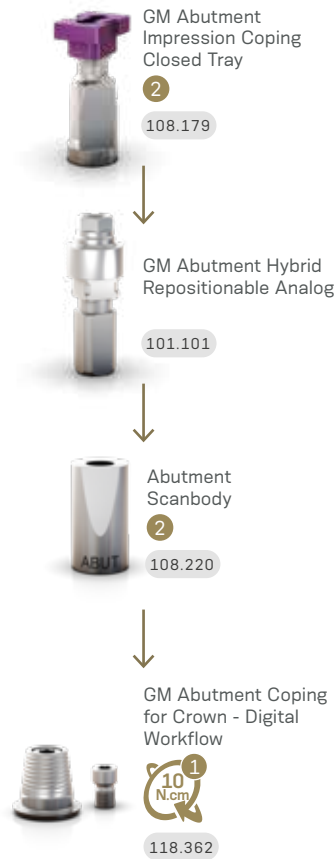


Conventional



Drivers



Accessories

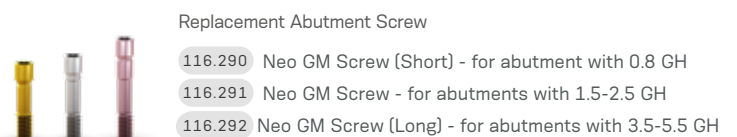

*Application of a film carbon-based coat that provides a lower friction coefficient, resulting in increased pre-load.

GM Mini Conical Abutment



Multiple-unit
screw-retained
prosthesis



Ø 4.8 mm

Consider in addition 1.5 - 2.0
mm for the restorative material;

Minimum interocclusal space of 4.5 mm from
the mucosa level for straight abutments;

Exact;

Neo Removable Screw.



Installation Sequence






Intraoral



Model Scanning






Conventional

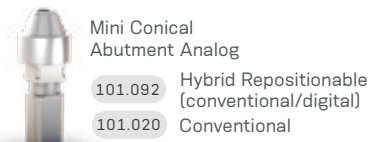

Drivers



Accessories



*Application of a film carbon-based coat that provides a lower friction coefficient, resulting in increased pre-load.

GM Micro Abutment

Consider in addition
1.5 - 2.0 mm for the
restorative material;

Minimum interocclusal
space of 3.5 mm from the
mucosa level.



Single-unit
screw-retained
prosthesis



Multiple-unit
screw-retained
prosthesis



Ø 3.5 mm



Recommended for limited spaces and narrow inter-dental spaces.

Installation Sequence

0.8 mm	1.5 mm	2.5 mm	GM Micro Abutment
115.255	115.256	115.257	
3.5 mm	4.5 mm	5.5 mm	
115.258	115.259	115.260	




Intraoral



Model Scanning



Conventional

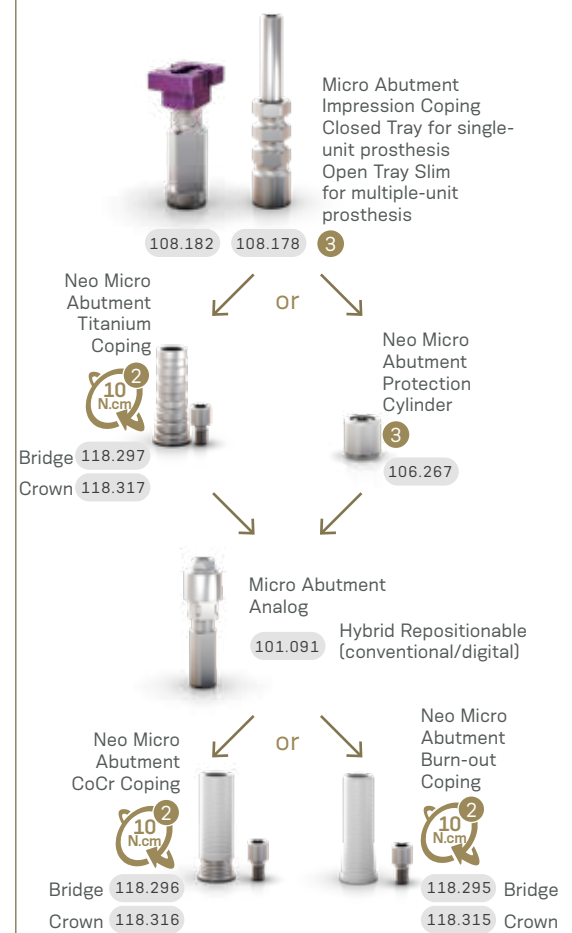

Drivers

- 1 Hexagonal Prosthetic Driver + Torque Wrench
- 2 Neo Screwdriver Torque Connection + Torque Wrench
- 3 Neo Screwdriver Torque Connection + Manual Screwdriver Torque

Accessories

- Micro Abutment Polishing Protector (123.015) Bridge
- Replacement Coping Screw (116.269) Titanium (116.270) Neotorque*

*Application of a film carbon-based coat that provides a lower friction coefficient, resulting in increased pre-load.

GM Anatomical Abutment



Single-unit
cement-retained
prosthesis

Recommended for anterior region.

Gingiva color for
esthetic outcomes;

Click retention for
provisional copings;

With internal threads for a secure
engagement of the screw;

Exact;

Neo Removable Screw.



Installation Sequence

In Mouth

GM Exact Click Anatomical Abutment with Neo Removable Screw

1 20 N.cm

1.5 mm	2.5 mm	3.5 mm
114.862	114.863	114.864
17°	114.865	114.866


or

GM Exact Click Narrow Anatomical Abutment with Neo Removable Screw

1 20 N.cm

1.5 mm	2.5 mm	3.5 mm
114.868	114.869	114.870
17°	114.871	114.872
		114.873

GM Exact Click Anatomical Abutment Provisional Coping



Impression of the GM Exact Click Anatomical Abutment

Lab stage

Finalized prosthesis

In Lab

GM Implant Exact Impression Coping Closed and Open Tray

2

Regular	108.160	108.162
Long	108.161	108.163

GM Implant Analog

Ø 3.5/3.75	Ø 4.0/4.3	Ø 5.0/6.0	Hybrid Repositionable (conventional/digital)
101.103	101.089	101.090	

GM Exact Click Anatomical Abutment Provisional Coping

118.334

118.335 Narrow

GM Exact Click Anatomical Abutment with Neo Removable Screw

1 20 N.cm

1.5 mm	2.5 mm	3.5 mm
114.862	114.863	114.864
17°	114.865	114.866

or

GM Exact Click Narrow Anatomical Abutment with Neo Removable Screw

1 20 N.cm

1.5 mm	2.5 mm	3.5 mm
114.868	114.869	114.870
17°	114.871	114.872
		114.873

Drivers

1 Neo Screwdriver Torque Connection + Torque Wrench

2 Neo Screwdriver Torque Connection + Manual Screwdriver Torque

Accessories

Replacement Abutment Screw

116.291 Neo GM Screw - for abutments with 0.8-2.5 GH

116.292 Neo GM Screw (Long) - for abutments with 3.5-5.5 GH

GM Universal Abutment



Single-unit
cement-retained
prosthesis




Ø 3.3/4.5 mm

Cementable area: 4.0 or 6.0 mm;
Click retention for provisional copings;
With internal threads for a secure engagement of the screw;
Exact;
Neo Removable Screw.



Installation Sequence



GM Exact Click
Universal Abutment with
Removable Screw



	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm
4 mm Ø 3.3	114.826	114.827	114.828	114.829	114.830	114.831
4 mm Ø 4.5	114.838	114.839	114.840	114.841	114.842	114.843
6 mm Ø 3.3	114.832	114.833	114.834	114.835	114.836	114.837
6 mm Ø 4.5	114.844	114.845	114.846	114.847	114.848	114.849

or



GM Exact Click
Universal Abutment 17°
with Removable Screw

	1.5 mm	2.5 mm	3.5 mm
4 mm Ø 3.3	114.802	114.803	114.804
4 mm Ø 4.5	114.808	114.809	114.810
6 mm Ø 3.3	114.805	114.806	114.807
6 mm Ø 4.5	114.811	114.812	114.813

or



GM Exact Click
Universal Abutment 30°
with Removable Screw

	1.5 mm	2.5 mm	3.5 mm
4 mm Ø 3.3	114.814	114.815	114.816
4 mm Ø 4.5	114.820	114.821	114.822
6 mm Ø 3.3	114.817	114.818	114.819
6 mm Ø 4.5	114.823	114.824	114.825

Intraoral



Universal Abutment
Intraoral Scanbody

4 mm Ø 3.3	108.143	6 mm Ø 3.3	108.144
4 mm Ø 4.5	108.145	6 mm Ø 4.5	108.146



Universal abutment Hybrid
Repositionable analog

4 mm Ø 3.3	101.097	6 mm Ø 3.3	101.098
4 mm Ø 4.5	101.099	6 mm Ø 4.5	101.100

Milled crown

Conventional



Click Universal
Abutment
Impression Coping

4 mm Ø 3.3	108.172	6 mm Ø 3.3	108.173
4 mm Ø 4.5	108.174	6 mm Ø 4.5	108.175



Click Universal
Abutment
Provisional Coping

4 mm Ø 3.3	118.304	6 mm Ø 3.3	118.305
4 mm Ø 4.5	118.306	6 mm Ø 4.5	118.307



Universal Abutment
Analog

4 mm Ø 3.3	101.097	6 mm Ø 3.3	101.098	Hybrid Repositionable (conventional/digital)
4 mm Ø 4.5	101.099	6 mm Ø 4.5	101.100	



Universal Abutment
Burn-out Coping

4 mm Ø 3.3	118.181	6 mm Ø 3.3	118.182
4 mm Ø 4.5	118.183	6 mm Ø 4.5	118.184

Drivers

1



Neo
Screwdriver
Torque
Connection

+



Torque Wrench

Accessories



Replacement
Abutment Screw

116.291 Neo GM Screw - for abutments with 0.8-2.5 GH

116.292 Neo GM Screw (Long) - for abutments with 3.5-5.5 GH

GM Titanium Base



Single-unit screw-retained prosthesis



Single-unit cement-retained prosthesis




Ø 3.5/4.5/
5.5/6.5 mm

Customizable up to 4 mm high;
Cementable area: 6.0 or 4.0 mm;
With internal threads for a secure engagement of the screw
Exact;
Neo Removable screw;



Installation Sequence

Intraoral





Model Scanning



GM Implant Exact Impression Coping Closed and Open Tray ²

Regular 108.160 108.162
Long 108.161 108.163



Conventional



GM Implant Exact Impression Coping Closed and Open Tray ²

Regular 108.160 108.162
Long 108.161 108.163



GM Exact Titanium Base with Removable Screw 4mm

	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm
Ø 3.5	135.355	135.356	135.357	135.358	135.359
Ø 4.5	135.367	135.368	135.369	135.370	135.371
Ø 5.5	135.379	135.380	135.381	135.382	135.383
Ø 6.5		135.391	135.392	135.393	135.394



GM Exact Titanium Base with Removable Screw 6mm

	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm
Ø 3.5	135.361	135.362	135.363	135.364	135.365
Ø 4.5	135.373	135.374	135.375	135.376	135.377
Ø 5.5	135.385	135.386	135.387	135.388	135.389
Ø 6.5		135.395	135.396	135.397	135.398




GM Titanium Base Burn-out Coping

	Ø 3.5	Ø 4.5	Ø 5.5
	118.322	118.325	118.329
	118.323	118.327	118.342

Drivers



Accessories



GM Titanium Base for Bridge



Multiple-unit
screw-
retained
prosthesis



Multiple-unit
cement-
retained
prosthesis



Ø 3.5/4.5/
5.5 mm


Cementable area:
4.0 mm for Ø 3.5
4.5 mm for Ø 4.5
and Ø 5.5.

With internal threads for a
secure engagement of the
screw;


Neo Removable Screw.



Intraoral



GM Implant
Intraoral
Scanbody
2
108.207

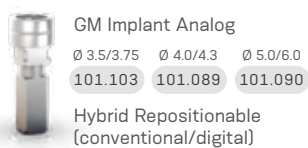

GM Implant Analog
Ø 3.5/3.75 Ø 4.0/4.3 Ø 5.0/6.0
101.103 101.089 101.090
Hybrid Repositionable
(conventional/digital)

Model Scanning



GM Implant Exact
Impression Coping
Open Tray
2
Regular 108.158
Long 108.159



GM Implant Analog
Ø 3.5/3.75 Ø 4.0/4.3 Ø 5.0/6.0
101.103 101.089 101.090
Hybrid Repositionable
(conventional/digital)



GM Implant
Intraoral
Scanbody
2
108.207



GM Titanium
Base for
Bridge
1
20 Ncm

	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm
Ø 3.5	135.399	135.400	135.401	135.402	135.403
Ø 4.5	135.404	135.405	135.406	135.407	135.408
Ø 5.5	135.409	135.410	135.411	135.412	135.413

Drivers

1



Neo
Screwdriver
Torque
Connection

+



Torque Wrench

2



Neo
Screwdriver
Torque
Connection

+



Manual
Screwdriver
Torque

Accessories



Replacement Abutment
Screw

116.292 Neo GM Screw (Long)

GM Titanium Base Angled Solution (AS)

 Single-unit screw-retained prosthesis
  Single-unit cement-retained prosthesis
  Ø 4.0/4.5/5.5 mm

With removable screw.


Cementable area:
6.0 or 4.0 mm;

Exact.




Installation Sequence


Intraoral

 GM Implant Intraoral Scanbody
 108.207

↓


 GM Implant Analog
 Ø 3.5/3.75 Ø 4.0/4.3 Ø 5.0/6.0
 101.103 101.089 101.090
 Hybrid Repositionable (conventional/digital)

Model Scanning


 GM Implant Exact Impression Coping
 Closed and Open Tray 2

Regular 108.160 108.162
 Long 108.161 108.163

↓

 GM Implant Analog
 Ø 3.5/3.75 Ø 4.0/4.3 Ø 5.0/6.0
 101.103 101.089 101.090
 Hybrid Repositionable (conventional/digital)

↓

 GM Implant Intraoral Scanbody
 108.207

	0.8 mm	1.5 mm	2.5 mm							
Ø 4.0	135.327	135.328	135.329	 GM Titanium Base Angled Solution (AS) 4mm  GM Titanium Base Angled Solution (AS) 6mm	or	 GM Titanium Base Angled Solution (AS) 6mm	0.8 mm	1.5 mm	2.5 mm	
Ø 4.5	135.333	135.334	135.335		Ø 4.0		135.330	135.331	135.332	
Ø 5.5	135.339	135.340	135.341		Ø 4.5		135.336	135.337	135.338	
							Ø 5.5	135.342	135.343	135.344

Drivers

 Angled Solution Screwdriver for Torque Wrench
 105.150 Short
 105.151 Regular
 105.152 Long

+



 Torque Wrench

or


 Angled Solution Screwdriver for Contra-angle
 105.147 Short
 105.148 Regular
 105.149 Long

+

 Contra-angle

 Neo Screwdriver Torque Connection
 +
 Manual Screwdriver Torque

Accessories

 Replacement Sterile Screw
 116.288 Screw for GM Titanium Base AS

Titanium Base C for GM



Single-unit screw-retained prosthesis



Single-unit cement-retained prosthesis



Ø 4.65 mm

Cementable area: 4.7 mm;


With internal threads for a secure engagement of the screw;

Exact;

Neo Removable Screw.



Installation Sequence

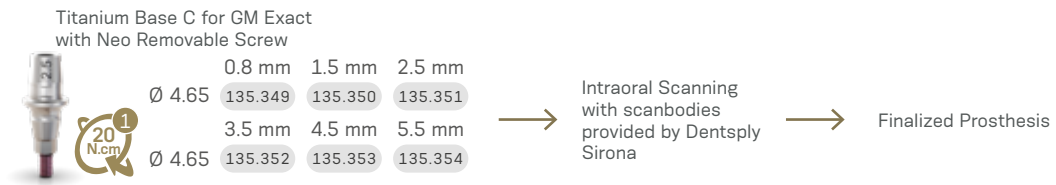

Workflow

Step 1

Gingiva height selection and ordering.



Select the Titanium Base C for GM Exact gingival height.



Order the Titanium Base C for GM Exact. Please note that the scanbody has to be purchased directly from equipment manufacturer.

Step 2

Intra-oral scanning.



Insert the Titanium Base C for GM Exact in the Neodent® implant.



Insert scanbody on the Titanium Base C for GM Exact.

Step 3

Design and milling.



Select in the CAD software the comparable third-party Ti-base and perform the digital design.



Mill the digital design.

Step 4

Finalization and fixation.



- Check the fit of milled restoration in the patient's mouth and adapt it, if needed.
- Cement the restoration on the Titanium Base C for GM Exact and insert it into the patient's mouth.

CEREC digital library compatibility

Library	Sirona's Products				Compatible with implant System	
	Scanbody	REF Scanbody Omnicam	REF Scanbody Bluecam / Ineos	Grinding block	Implant manufacturer	Implant system
NBB 3.4 L						
NB A 4.5 L						
SSO 3.5 L						
S BL 3.3 L	L	6431329	6431303	inCoris ZI meso L	Neodent®	GM, CM, HE, IIPlus
S BL 4.1 L						
BO 3.4 L						

Drivers

1

Neo Screwdriver Torque Connection



Torque Wrench

Accessories



Replacement Abutment Screw

116.292 Neo GM Screw (Long)

GM Titanium Block for MEDENTiKA Holder



Single-unit screw-retained prosthesis



Single-unit cement-retained prosthesis



Multiple-unit cement-retained prosthesis



Ø 11.5/
15.8 mm

Screw sold separately.


Cementable area: 14.2 mm;

Exact.




Installation Sequence

Complete Digital Workflow

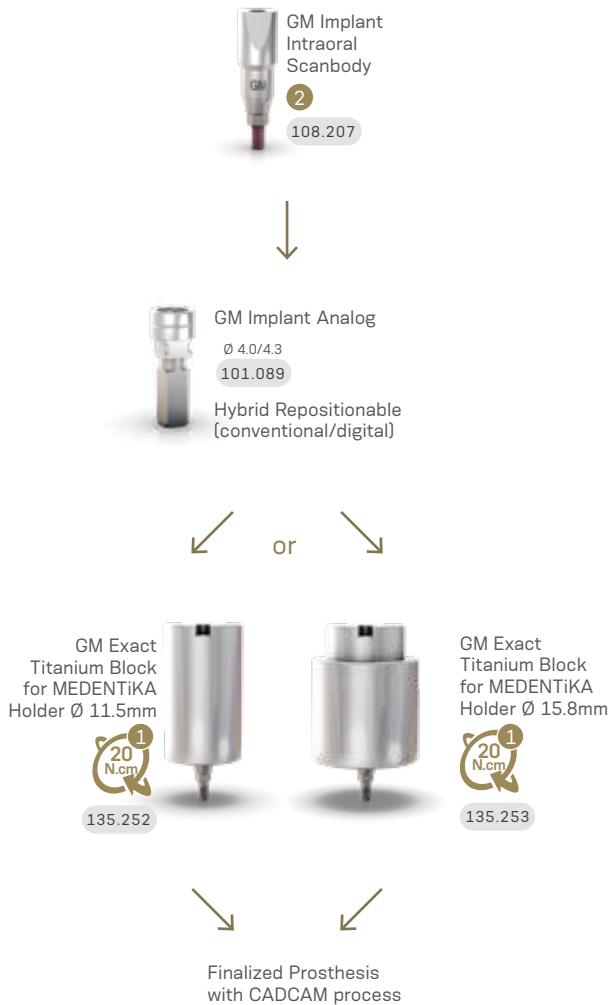

Semi Digital Workflow

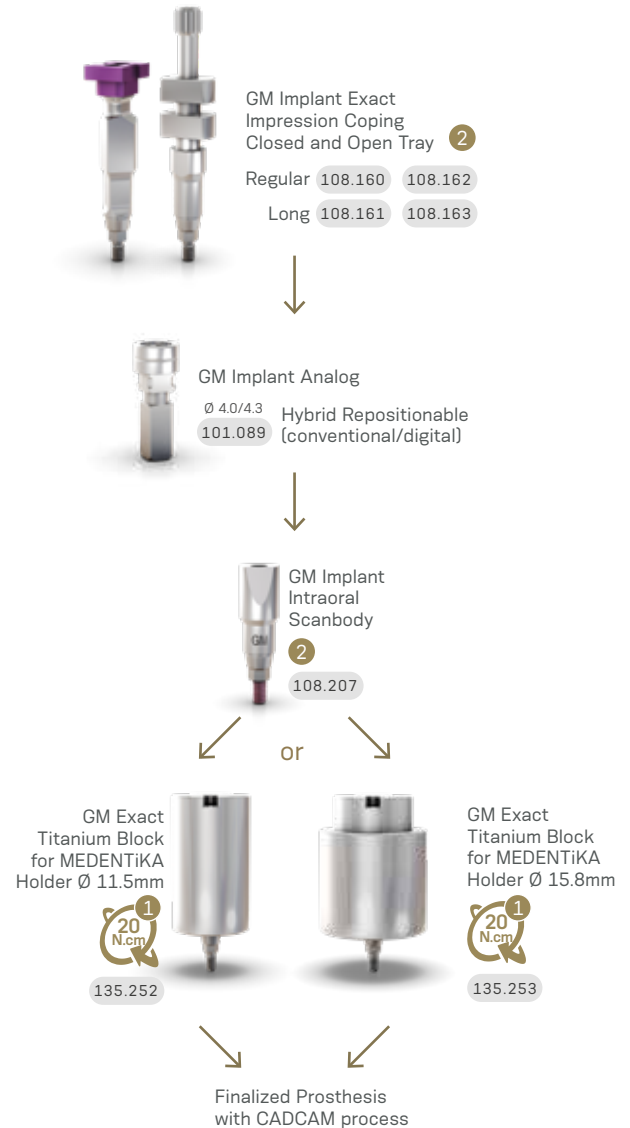

Drivers



Accessories



*Application of a film carbon-based coat that provides a lower friction coefficient, resulting in increased pre-load.

GM Titanium Block for AG Holder



Single-unit screw-retained prosthesis



Single-unit cement-retained prosthesis



Multiple-unit cement-retained prosthesis



Ø 12.0 mm

Screw sold separately.


Installation Sequence

Complete Digital Workflow



GM Implant Intraoral Scanbody

108.207



GM Implant Analog

Ø 4.0/4.3
101.089

Hybrid Repositionable (conventional/digital)



GM Exact Titanium Block for Amann Girschbach Holder
Ø 12.0mm

135.226



Finalized Prosthesis with CAD/CAM process

Semi Digital Workflow



GM Implant Exact Impression Coping Closed and Open Tray ²


Regular 108.160 108.162

Long 108.161 108.163



GM Implant Analog

Ø 4.0/4.3 Hybrid Repositionable (conventional/digital)
101.089



GM Implant Intraoral Scanbody

108.207



GM Exact Titanium Block for Amann Girschbach Holder
Ø 12.0mm

135.226



Finalized Prosthesis with CAD/CAM process

Drivers



Accessories



Sterile Screws sold separately

116.286 Titanium

116.285 Neotorque*

*Application of a film carbon-based coat that provides a lower friction coefficient, resulting in increased pre-load.

GM CoCr Abutment

Consider in addition 1.5 - 2.0 mm for the restorative material;

Interocclusal height of 12 mm (can be customized up to 5.0 mm);



Single-unit screw-retained prosthesis



Single-unit cement-retained prosthesis




Ø 4.1/4.5/
5.0 mm

For implants placed at bone level.

Exact.


Installation Sequence

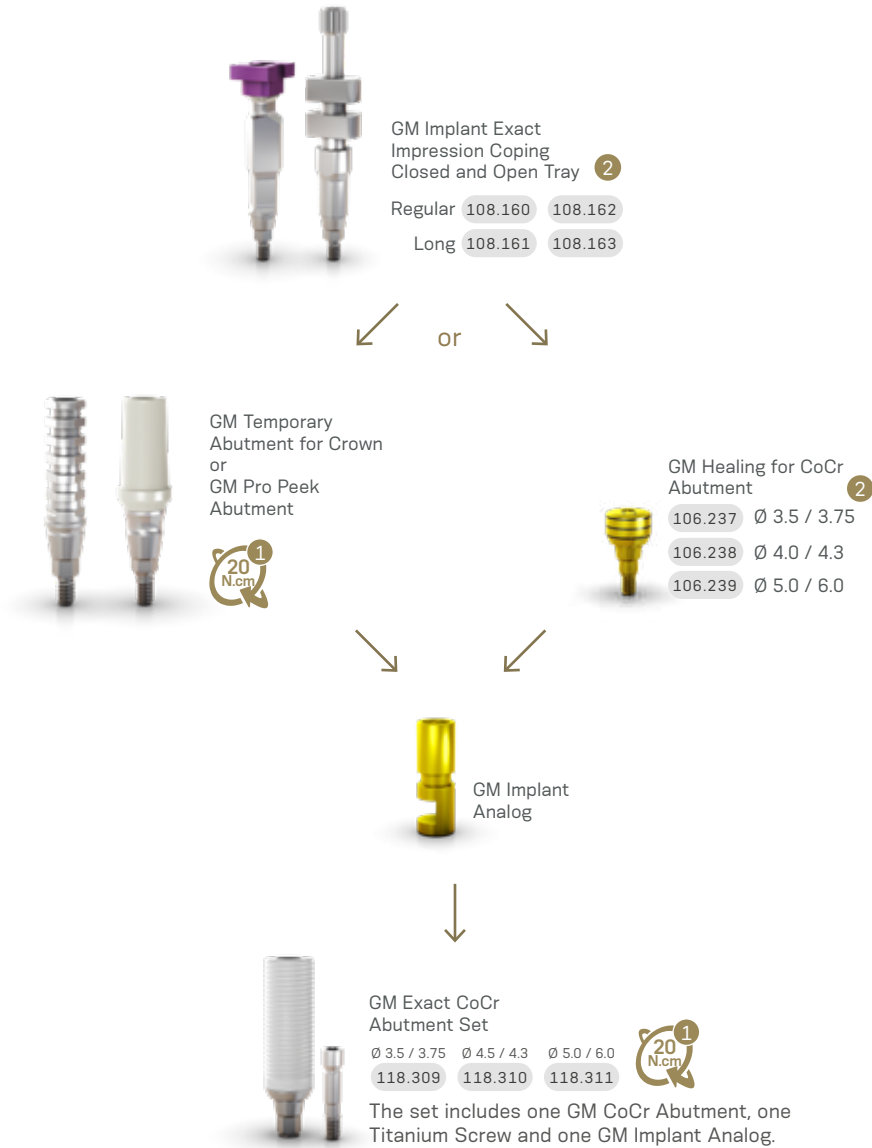

Drivers



Accessories



*Application of a film carbon-based coat that provides a lower friction coefficient, resulting in increased pre-load.

GM Temporary Abutment



Single-unit screw-retained temporary prosthesis



Multiple-unit screw-retained temporary prosthesis




Ø 3.5/
4.5 mm

Consider in addition 1.5 - 2.0 mm for the restorative material;

Channels of customizations;

Interocclusal height of 10 mm (can be customized up to 4.0 mm);

Exact.

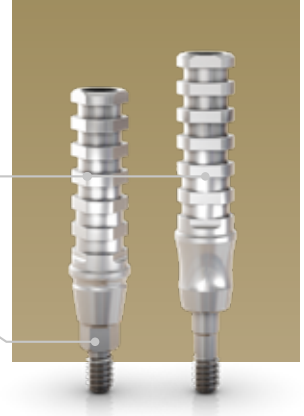


Customizable area made of titanium.

A minimum height of 4 mm of the customizable area must be kept.

With retentive grooves for acrylic material and allows customization.

Installation Sequence

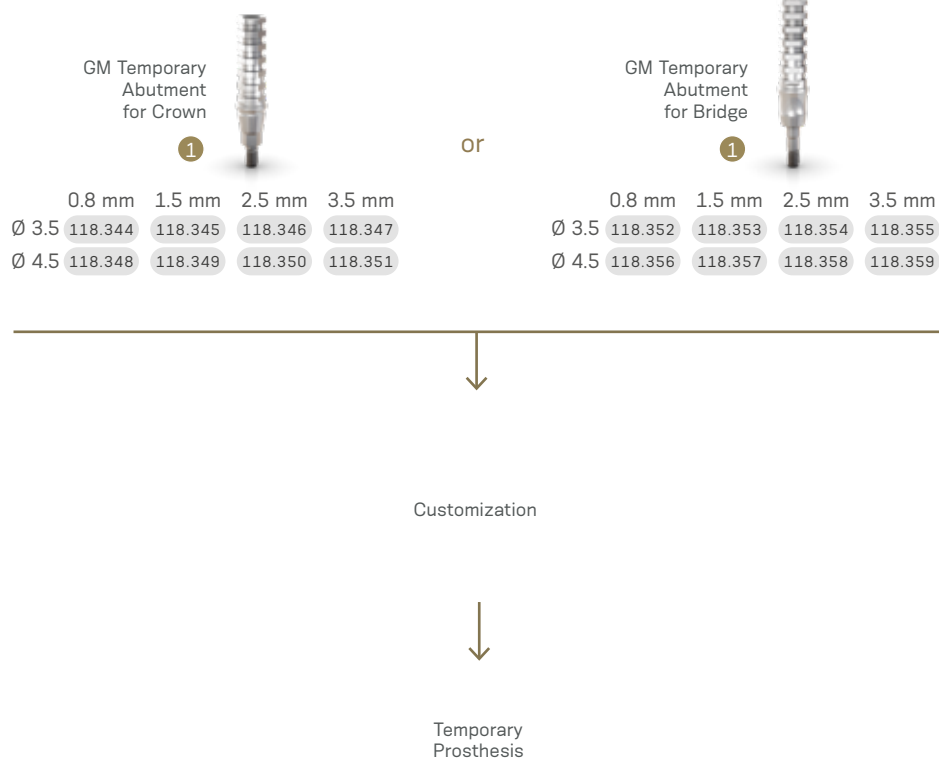

Drivers

1



Neo Screwdriver Torque Connection

+



Torque Wrench

Accessories



Replacement Sterile Screws

116.286 Titanium

116.285 Neotorque*

*Application of a film carbon-based coat that provides a lower friction coefficient, resulting in increased pre-load.

GM Pro Peek Abutment



Single-unit
cement-retained
temporary
prosthesis



Ø 4.5/
6.0 mm

Biocompatible Peek of easy customization.

Consider in addition 1.5 - 2.0 mm
for the restorative material;


Interocclusal height of 9.2
mm (can be customized up
to 5.0 mm);

With internal threads for a
secure engagement of the
screw;

Exact;
Neo Removable Screw.




Installation Sequence

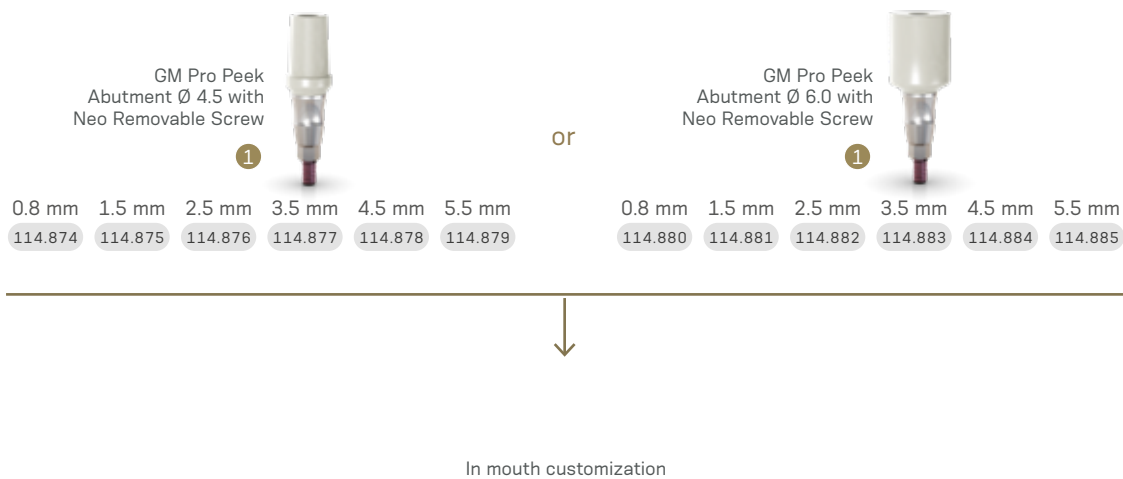

Drivers



Accessories

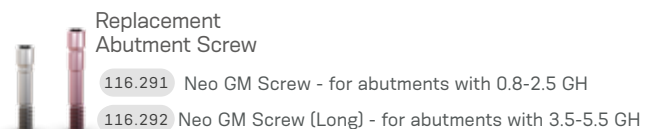

GM Novaloc




Overdenture


Angled version with removable screw.



Installation Sequence

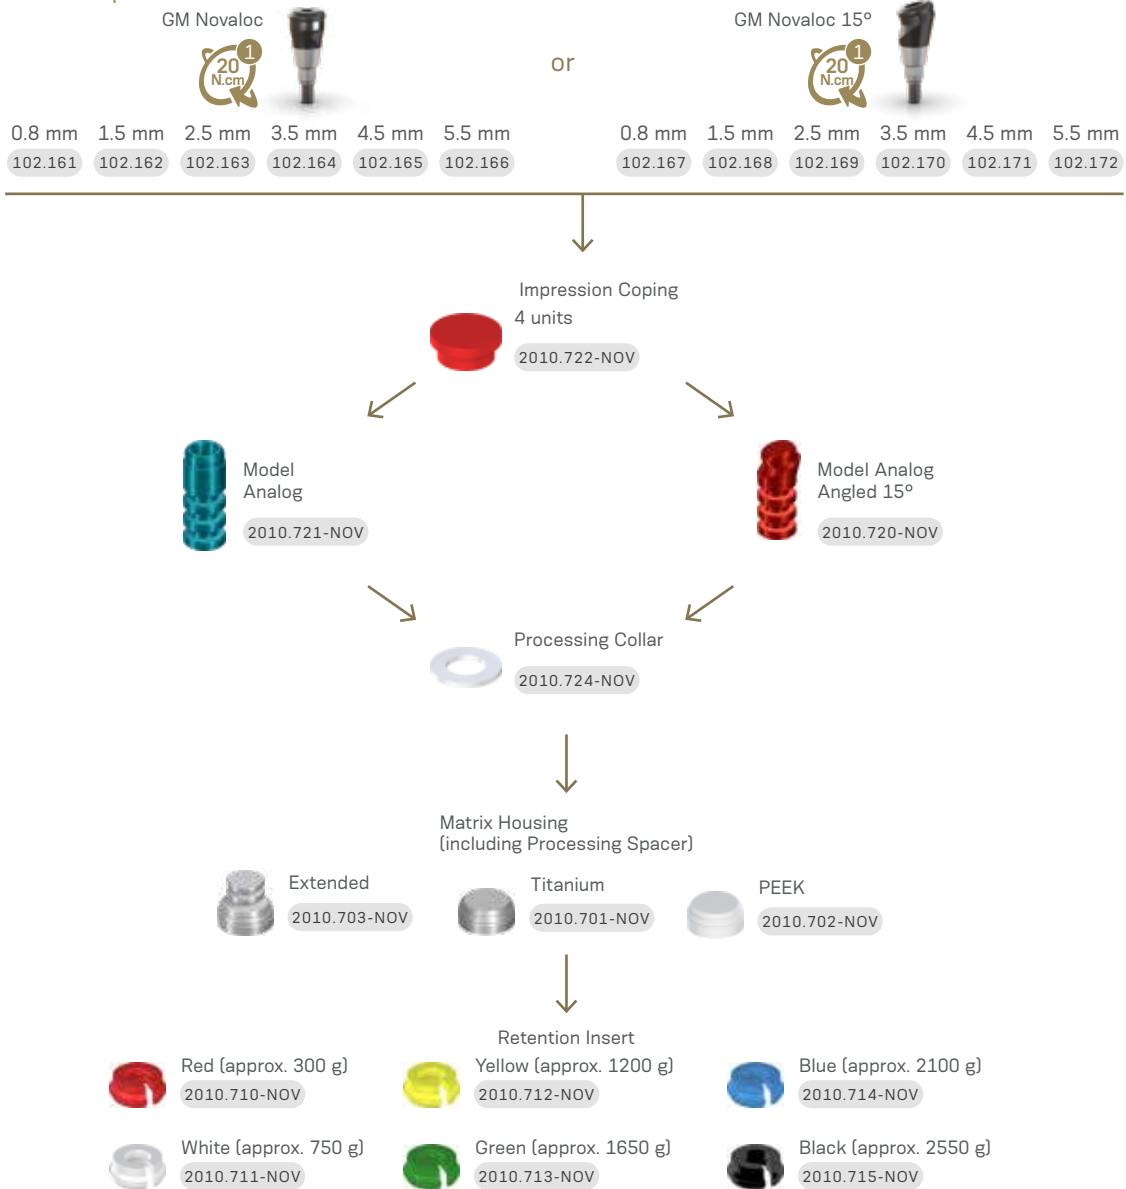

Drivers




Accessories




Measurements GM Mini Conical Abutment

17°

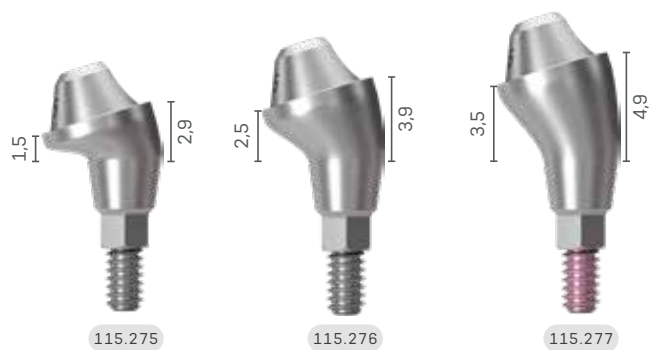


Measurements GM Anatomic Abutment

Narrow Anatomic
Abutment

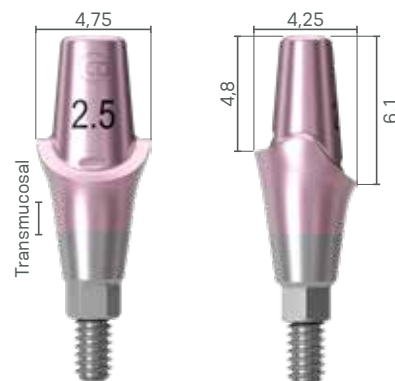


Anatomic
Abutment

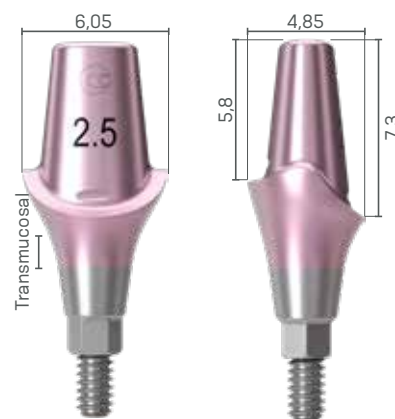

30°



Narrow Anatomic Abutment 17°

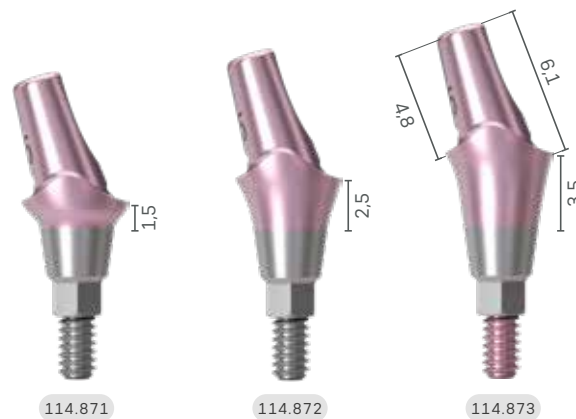

Anatomic Abutment 17°




Measurements GM Universal Abutment


4 mm chimney height / \varnothing 3.3 / 17°




4 mm chimney height / \varnothing 3.3 / 30°

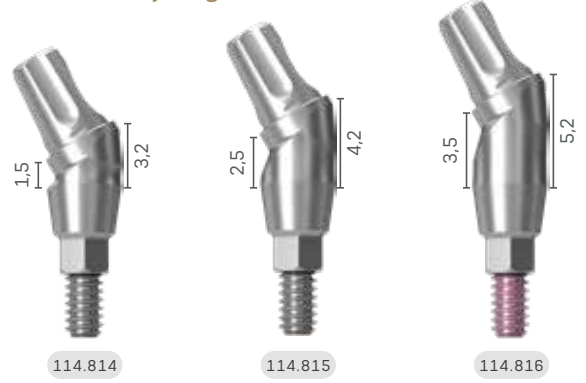


4 mm chimney height / \varnothing 4.5 / 17°

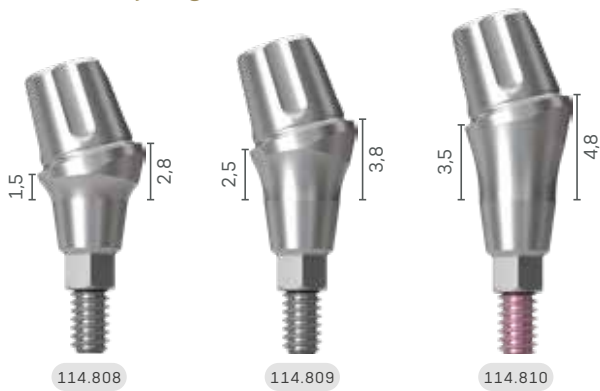


4 mm chimney height / \varnothing 4.5 / 30°

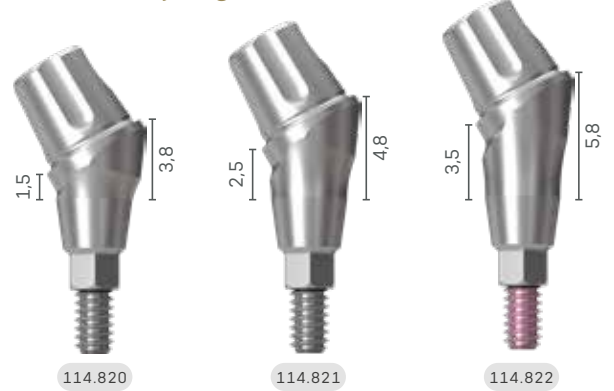

6 mm chimney height / \varnothing 3.3 / 17°

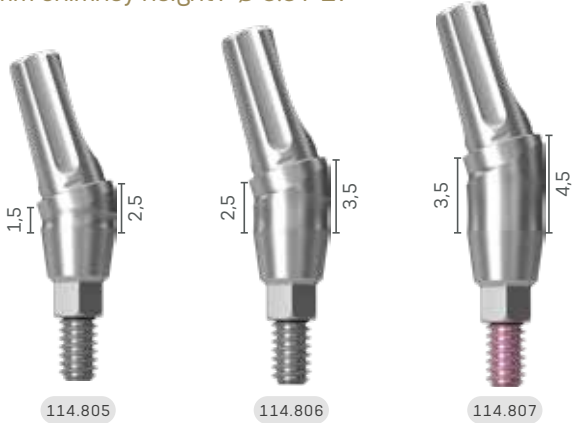


6 mm chimney height / \varnothing 3.3 / 30°

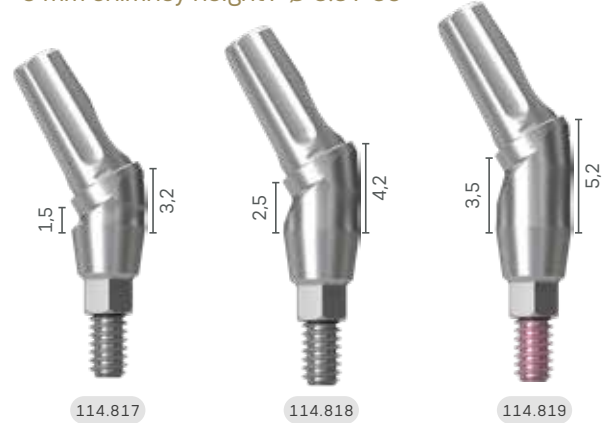

6 mm chimney height / \varnothing 4.5 / 17°



6 mm chimney height / \varnothing 4.5 / 30°

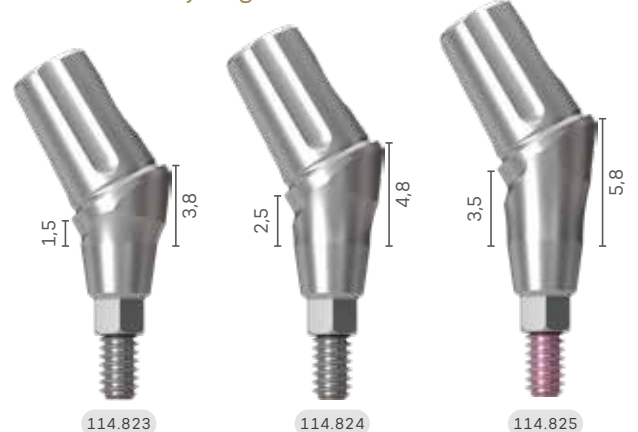

Grand Morse® Kits

Grand Morse® Surgical Kit

Autoclavable polymer case.

To order the pre-mounted version of the kit, with its complete composition with non-color coded drills, use code [110.302](#).



Articles

- 110.288 GM Surgical Kit Case
- 103.162 Twist Drill 2.0 Plus
- 103.213 Pilot Drill 2.0/3.0 Plus
- 103.164 Twist Drill 3.0 Plus
- 103.166 Twist Drill 3.3 Plus
- 103.167 Twist Drill 3.8 Plus
- 103.168 Twist Drill 4.3 Plus
- 103.163 Twist Drill 2.8 Plus
- 103.170 Initial Drill Plus
- 103.513 Pilot Drill GM 2.8/3.5
- 103.514 Pilot Drill GM 3.0/3.75
- 103.515 Pilot Drill GM 3.3/4.0
- 103.516 Pilot Drill GM 4.3
- 103.517 Pilot Drill GM 4.3/5.0


- 103.578 Tapered Contour Drill 3.5
- 103.579 Tapered Contour Drill 3.75
- 103.580 Tapered Contour Drill 4.0
- 103.581 Tapered Contour Drill 4.3
- 103.582 Tapered Contour Drill 5.0
- 103.425 Tapered Drill 2.0
- 103.561 Tapered Drill 3.5
- 103.564 Tapered Drill 3.75
- 103.567 Tapered Drill 4.0
- 103.570 Tapered Drill 4.3
- 103.573 Tapered Drill 5.0
- 103.576 Tapered Drill 6.0
- 105.131 GM Implant Driver - Contra-Angle
- 104.060 Neo Screwdriver (Medium)

- 105.130 GM Implant Driver - Torque Wrench (Long)
- 104.028 Manual Implant Driver - Contra-Angle
- 105.129 GM Implant Driver - Torque Wrench (Short)
- 128.019 Direction Indicator 2.8/3.5
- 128.020 Direction Indicator 3.0/3.75
- 128.021 Direction Indicator 3.3/4.0
- 128.022 Direction Indicator 3.6/4.3
- 128.023 Direction Indicator 4.3/5.0
- 128.028 Height Measurer GM
- 129.004 Depth Probe
- 129.001 Titanium Tweezers
- 104.050 Torque Wrench
- 103.426 Drill Extension

Note: Items that compose Neodent® Kits are sold separately.

Grand Morse® and WS Surgical Kit

Autoclavable polymer case.

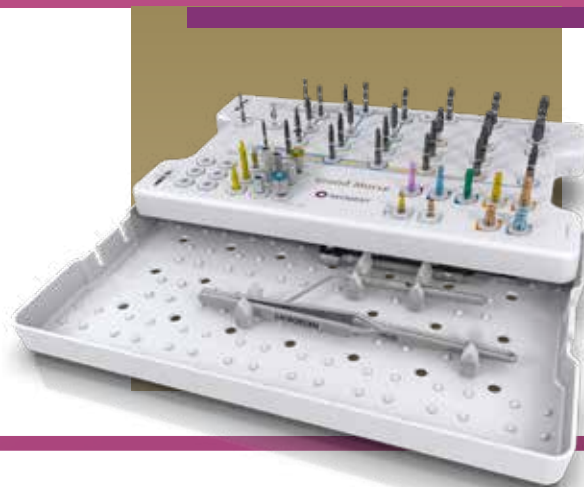

Articles

- 110.287 GM/WS Surgical Kit Case
- 103.162 Twist Drill 2.0 Plus
- 103.213 Pilot Drill 2.0/3.0 Plus
- 103.164 Twist Drill 3.0 Plus
- 103.166 Twist Drill 3.3 Plus
- 103.514 GM Pilot Drill 3.0/3.75
- 103.167 Twist Drill 3.8 Plus
- 103.168 Twist Drill 4.3 Plus
- 103.215 Pilot Drill 4.3/5.3 Plus
- 103.163 Twist Drill 2.8 Plus
- 103.169 Twist Drill 5.3 Plus
- 103.170 Initial Drill Plus
- 103.513 Pilot Drill GM 2.8/3.5
- 103.515 Pilot Drill GM 3.3/4.0
- 103.516 Pilot Drill GM 4.3
- 103.517 Pilot Drill GM 4.3/5.0
- 103.221 Pilot Drill CM 5.3/6.0 Plus

- 103.578 Tapered Contour Drill 3.5
- 103.579 Tapered Contour Drill 3.75
- 103.580 Tapered Contour Drill 4.0
- 103.581 Tapered Contour Drill 4.3
- 103.582 Tapered Contour Drill 5.0
- 103.425 Tapered Drill 2.0
- 103.561 Tapered Drill 3.5
- 128.029 WS Height Measurer
- 103.564 Tapered Drill 3.75
- 103.567 Tapered Drill 4.0
- 103.570 Tapered Drill 4.3
- 103.573 Tapered Drill 5.0
- 103.576 Tapered Drill 6.0
- 105.131 GM Implant Driver - Contra-Angle
- 105.002 Smart/WS Implant Driver - Contra-Angle
- 104.060 Neo Screwdriver (Medium)
- 105.130 GM Implant Driver GM - Torque Wrench

- 105.018 Hex Connection - Torque Wrench (Long)
- 104.028 Manual Implant Driver - Contra-Angle
- 104.012 Manual Screwdriver (Medium)
- 105.129 GM Implant Driver GM - Torque Wrench
- 105.001 Smart/WS Implant Driver - Torque Wrench (Short)
- 128.019 Direction Indicator 2.8/3.5
- 128.020 Direction Indicator 3.0/3.75
- 128.021 Direction Indicator 3.3/4.0
- 128.022 Direction Indicator 3.6/4.3
- 128.023 Direction Indicator 4.3/5.0
- 128.024 WS Direction Indicator 4.3/5.0
- 128.025 WS Direction Indicator 5.3/6.0
- 128.028 GM Height Measurer
- 129.004 Depth Probe
- 129.001 Titanium Tweezers
- 104.050 Torque Wrench
- 103.426 Drill Extension

Note: Items that compose Neodent® Kits are sold separately.

Helix GM[®] Compact Surgical Kit

Autoclavable polymer case.

The Kit allows the installation of Helix GM[®] Implants in all bone types.

To order the pre-mounted version of the kit, with its complete composition with non-color coded drills, use code [110.303](#).



Articles

- 110.297 Helix GM[®] Compact Surgical Kit Case
- 103.170 Initial Drill
- 103.425 Tapered Drill 2.0
- 103.561 Tapered Drill 3.5
- 103.564 Tapered Drill 3.75
- 103.567 Tapered Drill 4.0
- 103.570 Tapered Drill 4.3
- 103.573 Tapered Drill 5.0
- 103.576 Tapered Drill 6.0
- 103.577 Tapered Drill 7.0 (Short)*
- 104.060 Neo Manual Screwdriver (Medium)
- 104.028 Manual Implant Driver - Contra-angle
- 103.426 Drill Extension
- 103.578 Tapered Contour Drill 3.5
- 103.579 Tapered Contour Drill 3.75
- 103.580 Tapered Contour Drill 4.0
- 103.581 Tapered Contour Drill 4.3
- 103.582 Tapered Contour Drill 5.0

- 105.131 GM Implant Driver - Contra-angle
- 105.130 GM Implant Driver - Torque Wrench (Long)
- 105.129 GM Implant Driver - Torque Wrench (Short)
- 103.513 GM Pilot Drill 2.8/3.5
- 103.514 GM Pilot Drill 3.0/3.75
- 103.515 GM Pilot Drill 3.3/4.0
- 103.516 GM Pilot Drill 4.3
- 103.517 GM Pilot Drill 4.3/5.0
- 128.028 GM Height Measurer
- 128.030 Angle Measurer for Drill 2.0 17°
- 128.031 Angle Measurer for Drill 2.0 30°
- 128.019 Direction Indicator 2.8/3.5
- 128.020 Direction Indicator 3.0/3.75
- 128.021 Direction Indicator 3.3/4.0
- 128.022 Direction Indicator 3.6/4.3
- 128.023 Direction Indicator 4.3/5.0
- 129.004 Depth Probe
- 104.050 Torque Wrench

Note: Items that compose Neodent[®] Kits are sold separately.

*Tapered Drill 7.0 is not included in the pre-mounted kit composition (110.303).



Neodent controlsystem



TRUST YOURSELF

The surgical procedure for implant placement can be perceived as complex, especially when performed in the posterior regions with limited visibility, or in proximity with anatomical structures such as nerve canals. The Neodent® Control System brings confidence and efficiency building trust during the surgical procedure.

Protect anatomical structures

The placement of implants requires accuracy, and the Neodent® Control System has been designed to reduce the risk against overdrilling and protecting anatomical structures such as nerves, the sinus or adjacent roots by securing the final depth.

Master limited visibility

The Neodent® Control System helps to provide confidence during situations with reduced visibility due to adjacent teeth, limited mouth opening, blood, saliva, making it difficult to read the lines on a twisting drill by reaching the planned depth.



Intuitive solution

The Neodent® Control System is a color coded solution facilitating the identification of the drill sequence, the diameter and length of the implant and the combination of drill stop and drill.



Secure drill stop locking system

The Neodent® Control Drill Stop features a modern drill locking system enabling an easy and secure engaging into the drill, offering a peace-of-mind surgical experience.



Multiple use solution

The Neodent® Control Drill Stops are made of titanium for professional cleaning and autoclaving allowing multiple use.

User friendly kit retentive system

The Neodent® Control Drill Stop Kit includes an innovative retentive system.



A convenient and time-saving pick and drop mechanism during the surgical procedure.

Neodent® Color Code overview



Color code according to implant length



Compatible portfolio of Helix GM® Implants



Length	Diameter						
	3.5	3.75	4.0	4.3	5.0	6.0	7.0
8	✓	✓	✓	✓	✓	✓	✓
10	✓	✓	✓	✓	✓	✓	✓
11.5	✓	✓	✓	✓	✓	✓	✓
13	✓	✓	✓	✓	✓	✓	✓



DR ARANTZA RODRIGUEZ, from Spain

“Neodent®, compared to other brands, gives me security and long-term stability this is very confident for me and of course for my patient.”

Helix GM[®] Compact Kit Control Stop Drills

Autoclavable polymer case.

The Kit allows the installation of Helix GM[®] Implants in all bone types, using the Neodent[®] Control Stop Drills.

To order the pre-mounted version of the kit, with its complete composition, use code [110.308](#).



Articles

- 110.297 Helix GM[®] Compact Surgical Kit Case
- 103.170 Initial Drill
- 103.492 Tapered Control Stop Drill 2.0
- 103.493 Tapered Control Stop Drill 3.5
- 103.494 Tapered Control Stop Drill 3.75
- 103.495 Tapered Control Stop Drill 4.0
- 103.496 Tapered Control Stop Drill 4.3
- 103.497 Tapered Control Stop Drill 5.0
- 103.498 Tapered Control Stop Drill 6.0 (Short)
- 103.499 Tapered Control Stop Drill 7.0 (Short)*
- 104.060 Neo Manual Screwdriver (Medium)
- 104.028 Manual Implant Driver - Contra-angle

- 103.426 Drill Extension
- 103.500 Tapered Control Stop Drill 3.5+
- 103.501 Tapered Control Stop Drill 3.75+
- 103.502 Tapered Control Stop Drill 4.0+
- 103.503 Tapered Control Stop Drill 4.3+
- 103.504 Tapered Control Stop Drill 5.0+
- 105.131 GM Implant Driver - Contra-angle GM
- 105.130 Implant Driver - Torque Wrench (Long)
- 105.129 GM Implant Driver - Torque Wrench (Short)
- 103.513 Pilot Drill 3.5
- 103.514 Pilot Drill 3.75
- 103.515 Pilot Drill 4.0

- 103.516 Pilot Drill 4.3
- 103.517 Pilot Drill 5.0
- 128.028 GM Height Measurer
- 128.030 Angle Measurer for Drill 2.0 17°
- 128.031 Angle Measurer for Drill 2.0 30°
- 128.019 Direction Indicator 2.8/3.5
- 128.020 Direction Indicator 3.0/3.75
- 128.021 Direction Indicator 3.3/4.0
- 128.022 Direction Indicator 3.6/4.3
- 128.023 Direction Indicator 4.3/5.0
- 129.004 Depth Probe
- 104.050 Torque Wrench

Note: Items that compose Neodent[®] Kits are sold separately.

*Tapered Control Stop Drill 7.0 is not included in the pre-mounted kit composition (110.308).

Control Drill Stop Kit

Autoclavable polymer case.

The Kit allows the sterilization and engagement of Neodent[®] Control Drill Stops on the drills.

To order the pre-mounted version of the kit, with its complete composition, use code [110.306](#).



Articles

- 110.307 Control Drill Stop Kit Case
- 125.144 8.0 Control Drill Stop D2.0
- 125.145 10.0 Control Drill Stop D2.0
- 125.146 11.5 Control Drill Stop D2.0
- 125.147 13.0 Control Drill Stop D2.0
- 125.148 8.0 Control Drill Stop D3.5
- 125.149 10.0 Control Drill Stop D3.5
- 125.150 11.5 Control Drill Stop D3.5
- 125.151 13.0 Control Drill Stop D3.5
- 125.152 8.0 Control Drill Stop D3.75/4.0
- 125.153 10.0 Control Drill Stop D3.75/4.0
- 125.154 11.5 Control Drill Stop D3.75/4.0


- 125.155 13.0 Control Drill Stop D3.75/4.0
- 125.156 8.0 Control Drill Stop D4.3/5.0
- 125.157 10.0 Control Drill Stop D4.3/5.0
- 125.158 11.5 Control Drill Stop D4.3/5.0
- 125.159 13.0 Control Drill Stop D4.3/5.0
- 125.160 8.0 Control Drill Stop D6.0/7.0
- 125.161 10.0 Control Drill Stop D6.0/7.0
- 125.162 11.5 Control Drill Stop D6.0/7.0
- 125.163 13.0 Control Drill Stop D6.0/7.0

Note: Items that compose Neodent[®] Kits are sold separately.

Grand Morse® Prosthetic Kit

Autoclavable polymer case.

To order the pre-mounted version of the kit, with its complete composition, use code [110.304](#).

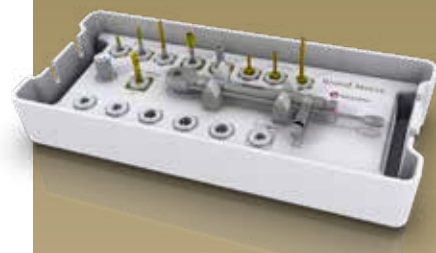

Articles

- 110.294 GM Prosthetic Kit Case
- 105.146 Neo Screwdriver Torque Connection - Contra-angle (Extra-short)
- 105.135 Neo Screwdriver Torque Connection - Contra-angle (Short)
- 105.136 Neo Screwdriver Torque Connection - Contra-angle (Medium)
- 105.138 Hexagonal Prosthetic Driver - Contra-angle
- 105.137 Hexagonal Prosthetic Driver - Torque Wrench
- 105.133 Neo Screwdriver Torque Connection (Short) - Torque Wrench
- 105.132 Neo Screwdriver Torque Connection (Medium) - Torque Wrench
- 105.157 Neo Long Screwdriver for Torque Wrench
- 104.005 Manual Screwdriver Torque
- 128.028 GM Height Measurer
- 104.050 Torque Wrench

Note: Items that compose Neodent® Kits are sold separately.

Grand Morse® Try-In Kit

Autoclavable polymer case.

To order the pre-mounted version of the kit, with its complete composition, use code [110.305](#).



Articles

- | | | |
|--------------------------------------|--|---|
| 110.295 GM Try-In Kit Case | 114.782 GM Abutment Try-In 4.5X6X4.5 | 114.793 GM Abutment Try-In 30° 4.5X6X1.5 |
| 114.772 GM Abutment Try-In 3.3X6X0.8 | 114.783 GM Abutment Try-In 4.5X6X5.5 | 114.794 GM Abutment Try-In 30° 4.5X6X2.5 |
| 114.773 GM Abutment Try-In 3.3X6X1.5 | 114.784 GM Abutment Try-In 17° 3.3X6X1.5 | 114.795 GM Abutment Try-In 30° 4.5X6X3.5 |
| 114.774 GM Abutment Try-In 3.3X6X2.5 | 114.785 GM Abutment Try-In 17° 3.3X6X2.5 | 114.796 GM Anatomic Abutment Try-In 1.5 |
| 114.775 GM Abutment Try-In 3.3X6X3.5 | 114.786 GM Abutment Try-In 17° 3.3X6X3.5 | 114.797 GM Anatomic Abutment Try-In 2.5 |
| 114.776 GM Abutment Try-In 3.3X6X4.5 | 114.787 GM Abutment Try-In 17° 4.5X6X1.5 | 114.798 GM Anatomic Abutment Try-In 3.5 |
| 114.777 GM Abutment Try-In 3.3X6X5.5 | 114.788 GM Abutment Try-In 17° 4.5X6X2.5 | 114.799 GM Lateral Anatomic Abutment Try-In 1.5 |
| 114.778 GM Abutment Try-In 4.5X6X0.8 | 114.789 GM Abutment Try-In 17° 4.5X6X3.5 | 114.800 GM Lateral Anatomic Abutment Try-In 2.5 |
| 114.779 GM Abutment Try-In 4.5X6X1.5 | 114.790 GM Abutment Try-In 30° 3.3X6X1.5 | 114.801 GM Lateral Anatomic Abutment Try-In 3.5 |
| 114.780 GM Abutment Try-In 4.5X6X2.5 | 114.791 GM Abutment Try-In 30° 3.3X6X2.5 | 104.058 Neo Manual Screwdriver (Short) |
| 114.781 GM Abutment Try-In 4.5X6X3.5 | 114.792 GM Abutment Try-In 30° 3.3X6X3.5 | 128.028 GM Height Measurer |

Note: Items that compose Neodent® Kits are sold separately.

Grand Morse® Instruments



Initial Drill

- :: Available in surgical steel;
- :: 2.0mm diameter.

103.170

Tapered Drills

- :: Available in surgical steel;
- :: Drill sequence for Helix GM® and Drive GM® Implants;
- :: With a color code according to the drill diameter.



	Short 31 mm	Regular 35 mm	Long 43 mm
Ø 2.0	103.559	103.425	103.560
Ø 3.5	103.562	103.561	103.563
Ø 3.75	103.565	103.564	103.566
Ø 4.0	103.568	103.567	103.569
Ø 4.3	103.571	103.570	103.572
Ø 5.0	103.574	103.573	103.575
Ø 6.0	103.576		
Ø 7.0	103.577		

Tapered+ Drills

- :: For preparing the implant bed in bone types I and II for Helix GM® Implants;
- :: With a color code according to the drill diameter and 2 stripes of color for identification.



Ø 3.5+	103.578
Ø 3.75+	103.579
Ø 4.0+	103.580
Ø 4.3+	103.581
Ø 5.0+	103.582

Pilot Drills

- :: Available in surgical steel;
- :: Increasing the surgical alveolus diameter ridge, easing the penetration of the next drill or the implant.



Ø 2/3	103.213		
Ø 3.5	103.513	Ø 5.0	103.517
Ø 3.75	103.514	Ø 3.8/4.3	103.214
Ø 4.0	103.515	Ø 4.3/5.3	103.215
Ø 4.3	103.516	Ø 5.3/6	103.221

Twist Drills

- :: Available in surgical steel;
- :: Drill sequence for Titamax GM® Implants.



	Short 31 mm	Regular 35 mm	Long 43 mm
Ø 2.0	103.222	103.162	103.228
Ø 2.8	103.223	103.163	103.229
Ø 3.0	103.224	103.164	103.230
Ø 3.3	103.225	103.166	103.231
Ø 3.8	103.226	103.167	
Ø 4.3	103.227	103.168	

Tapered Control Stop Drills



- :: Available in surgical steel;
- :: Drill sequence for Helix GM® Implants;
- :: Attachment to engage drill stops;
- :: With a color code according to the drill diameter.

Ø 2.0	103.492	Ø 4.3	103.496
Ø 3.5	103.493	Ø 5.0	103.497
Ø 3.75	103.494	Ø 6.0	103.498
Ø 4.0	103.495	Ø 7.0	103.499

Tapered+ Control Stop Drills



- :: Available in surgical steel;
- :: For preparing the implant bed in bone types I and II for Helix GM® Implants;
- :: Attachment to engage drill stops;
- :: With a color code according to the drill diameter and 2 stripes of color for identification.

Ø 3.5+	103.500	Ø 4.3+	103.503
Ø 3.75+	103.501	Ø 5.0+	103.504
Ø 4.0+	103.502		


Control Drill Stops

- :: Available in titanium;
- :: To be used in association with the Control Stop Drills;
- :: Physical control for drilling depth.

	8 mm	10 mm	11.5 mm	13 mm
Ø 2.0	125.144	125.145	125.146	125.147
Ø 3.5	125.148	125.149	125.150	125.151
Ø 3.75/4.0	125.152	125.153	125.154	125.155
Ø 4.3/5.0	125.156	125.157	125.158	125.159
Ø 6.0/7.0	125.160	125.161	125.162	125.163

Direction Indicators

- :: Available in titanium;
- :: Instrument to guide the implant position;
- :: Diameter of central band corresponds to GM Implant diameter;
- :: Smaller side to be used after Ø2.0mm drill;
- :: Larger side to be used after the last drill before implant installation.



2.8/3.5	128.019	3.6/4.3	128.022
3.0/3.75	128.020	4.3/5.0	128.023
3.3/4.0	128.021		

Drill Extension


- :: Available in surgical steel;
- :: Fit the drill directly into the Drill Extension.



103.426

GM Height Measurer

- :: Available in titanium;
- :: For selecting GM prosthetic abutments;
- :: Marks corresponding to transmucosa heights.
- :: Can be used as X-Ray Positioner.



128.028

GM Implant Driver - Contra-Angle



- :: To capture the implant directly from the packaging;
- :: To place GM Implants with contra-angle, or attached to a manual driver for contra-angle connections (104.028) for hand placement;
- :: With six dimples to indicate the hex index face position;
- :: The laser marks indicate the depth of implant placement, bone level, 1 and 2mm infra-bone and last marking (3mm) biological space;
- :: Maximum torque 35 N.cm.

105.131

GM Implant Driver - Torque Wrench



- :: To place GM Implants with the Torque Wrench (104.050);
- :: With six marks to indicate the hex index face position;
- :: The laser marks indicate the depth of implant placement, bone level, 1 and 2mm infra-bone and last marking (3mm) biological space;
- :: Maximum torque: 60 N.cm..

Short 22 mm	Long 30 mm
----------------	---------------

105.129 105.130

Neo Screwdriver Torque Connection - Torque Wrench



- :: Available in surgical steel;
- :: Yellow color for line identification.

Short 16.5 mm	Medium 22 mm	Long 32 mm
------------------	-----------------	---------------

105.133 105.132 105.157

Neo Manual Screwdriver



- :: Available in surgical steel;
- :: Yellow color for line identification

Short 21 mm	Medium 25 mm	Long 37 mm
----------------	-----------------	---------------

104.058 104.060 104.070

Neo Screwdriver Torque Connection - Contra-angle



- :: Available in surgical steel;
- :: Yellow color for line identification;
- :: Extra Short Neo Screwdriver Torque Connection - Contra-angle (105.146) recommended for Impression Copings, Cover Screws and Healing Abutments.

Extra Short 16.5 mm	Short 24 mm	Long 37 mm
------------------------	----------------	---------------

105.146 105.135 105.167

Hexagonal Prosthetic Driver



- :: Available in surgical steel;
- :: To install and apply torque over straight GM Mini Conical Abutments and GM Micro Abutments;

Contra-angle	Torque Wrench
--------------	---------------

105.138 105.137

Angled Solution Screwdriver for Torque Wrench



- :: To place GM Titanium Bases for Angled Solution with torque wrench;
- :: Maximum torque of 20 N.cm.

Short 16.5 mm	Medium 22.5 mm	Long 28.5 mm
------------------	-------------------	-----------------

105.150 105.151 105.152

Angled Solution Screwdriver for Contra-angle



- :: To place GM Titanium Bases for Angled Solution with contra-angle;
- :: Maximum torque of 20 N.cm.

Short 20 mm	Medium 26 mm	Long 32 mm
----------------	-----------------	---------------

105.147 105.148 105.149

GM Bone Profile Drill with Guide



- :: Available in surgical steel;
- :: Used in the surgical second step;
- :: Conforms the bone around the implant platform, preparing the emergence profile to be suitable to prosthetic components.

103.424

Angle Measurer for Drill 2.0



- :: Available in titanium;
- :: Angles: 17° and 30°;
- :: To select and plan the abutments angulation during surgical procedures;
- :: Suggested use: after Twist Drill 2.0.

17° 128.030	30° 128.031
----------------	----------------

GM Angle Measurer



- :: Available in titanium;
- :: Angles: 17° and 30°;
- :: To a more accurate selection and planning of the abutments angulation during the prosthetic phase.

17° 128.032	30° 128.033
----------------	----------------

Control Stop Kit Holder



- :: Available in polymer;
- :: Replacement piece;
- :: To keep the stops organized and to engage and remove them from the drills.

110.310

Manual Implant Drivers



- :: Available in surgical steel;
- :: For Contra-angle connections: connected to GM Implant Driver, it becomes a manual driver for implant placement.
- :: For Torque Wrench connections: connected to screwdrivers, it provides manual torque.

Contra-angle
Connections
104.028

Torque Wrench
Connections
104.005

Remover for Abutments with internal threads



- :: Available in surgical steel;
- :: To remove abutments with internal threads from the implants, after removal of the screws;
- :: Compatible with abutments with Neo removable Screws

130.118 Long
130.114

Remover for Neo Screws



- :: Available in surgical steel;
- :: Compatible with Neo removable screws for abutments

130.119 Long
130.115

Torque Wrench



- :: Available in surgical steel;
- :: Fitting for square connections;
- :: Collapsible Wrench that allows for proper assembly cleaning.

104.050

Removal Sets for Abutments with internal threads and Neo Screws

- :: Available in surgical steel;
- :: To remove Neo Removable Screws and abutments with internal threads from the implants, after removal of the screws;
- :: Compatible with abutments with Neo removable Screws



130.117

Long
130.116



Neodent easyguide

SIMPLICITY AT ONE HAND

Neodent® is designed to offer straightforward guided surgery techniques enabling predictable surgical results, efficient treatment protocols and patient treatment acceptance.



STRAIGHTFORWARD GUIDED SURGERY TECHNIQUE

Surgical convenience with one-hand procedures



EFFICIENT TREATMENT PROTOCOLS

Intuitive and simple technique



PREDICTABLE SURGICAL RESULTS

Confidence for accurate implant positioning



PATIENT TREATMENT ACCEPTANCE

Communication building trust and patient engagement



NEODENT® EASYGUIDE ENABLES ONE-HAND PROCEDURES WITH NO DRILL HANDLES

Simple technique

Reduced number of instruments

Surgeries can be performed without assistance

ONE DRILL DESIGN

The unique geometry of the Neodent® EasyGuide tapered drills is indicated for all bone types and dismisses the need for additional drill types or taps, simplifying the drilling sequence.



COLOR CODE ACCORDING TO IMPLANT DIAMETER



BUILT-IN TITANIUM STOP FOR PHYSICAL DEPTH CONTROL, WITH COLOR MATCHING THE SLEEVE IN THE SURGICAL GUIDE



LASER-MARKED LENGTH



ACTIVE PORTION MATCHING IMPLANT LENGTHS



DR FERNANDO DUQUE, from France

“The Easy Guide is easy to use, I think it’s completely friendly. The tools they provide us are easy to use and we can achieve excellent prosthetics and surgical outcomes with this. ”





FULLY GUIDED IMPLANT INSERTION


- Implant driver fits the sleeve, for a fully guided insertion with physical depth control;
- Offset: 10 mm.



FULLY GUIDED BED PREPARATION

- Intimate contact between drill and sleeve for accuracy in angulation;
- Depth control with stop drills,

1. DATA ACQUISITION
3D (CB)CT scan (DICOM)
Intraoral or lab scanning
(STL images)




2. VIRTUAL PLANNING
Implant positioned respecting the patient's anatomy and prosthetic outcome. Neodent® EasyGuide is compatible with major software.

3. SURGICAL GUIDE PRODUCTION
The surgical guide must contain the sleeves that guide the instruments and the implants.





4. SURGICAL PROCEDURE
Neodent® EasyGuide presents two surgical kits, selected according to the implant diameter.


EASYGUIDE KIT NARROW/REGULAR • Ø 3.5, Ø 3.75

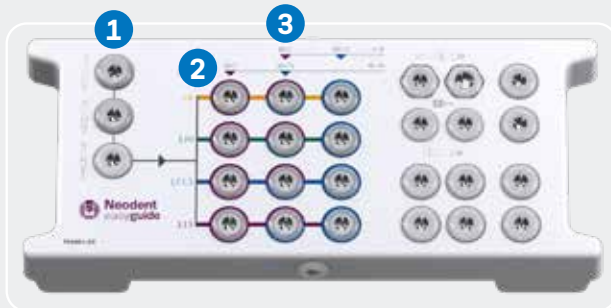

EASYGUIDE KIT REGULAR/WIDE • Ø 4.0, Ø 4.3, Ø 5.0

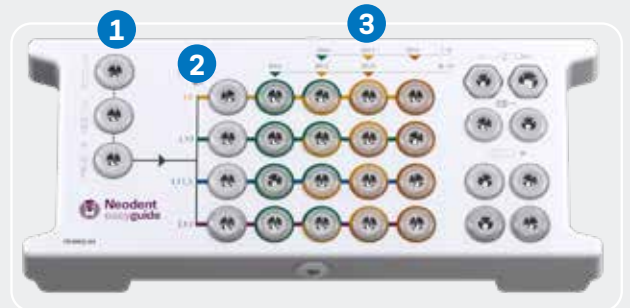

1
UNIQUE START
REGARDLESS
OF BONE TYPE



2
STRAIGHTFORWARD
IMPLANT LENGTH
IDENTIFICATION



3
COLOR CODED DRILL SEQUENCE FOR
EACH IMPLANT DIAMETER



NARROW SLEEVE: Ø3.5/Ø3.75



REGULAR SLEEVE: Ø4.0/Ø4.3/Ø5.0



DR MAJA CHMIELEWSKA, from Poland

"In the clinic, we do 100% of our surgeries guided, it's really helpful. The prosthodontic restoration in the end of the treatment, but also for patient comfort and for the fluency of our surgeries. I would strongly recommend to start this way! Easy Guides is very helpful and very fluent for our use and surgical practice."

Neodent®
EasyGuide
Kits

Neodent® EasyGuide Kit for Narrow/Regular Diameter Implants

Autoclavable polymer case.

The kit allows the installation of Helix GM® Implants of Ø3.5 and Ø3.75 in all bone types, using the Neodent® EasyGuide Guided Surgery Technique.



Articles

- 110.313 EasyGuide Kit Narrow/Reg. Diam. Tray
- 125.170 GM Narrow Stabilizer - 3 units per kit
- 105.161 GM Narrow Driver for Contra-angle
- 105.162 GM Narrow Driver for Torque Wrench
- 103.583 Narrow Mucosa Punch
- 103.519 Narrow Bone Leveling Drill
- 103.545 Narrow Initial Drill
- 103.546 Narrow Tapered Drill D3.5X8
- 103.547 Narrow Tapered Drill D3.5X10
- 103.548 Narrow Tapered Drill D3.5X11.5
- 103.549 Narrow Tapered Drill D3.5X13
- 103.550 Narrow Tapered Drill D3.5/3.75X8

- 103.551 Narrow Tapered Drill D3.5/3.75X10
- 103.552 Narrow Tapered Drill D3.5/3.75X11.5
- 103.553 Narrow Tapered Drill D3.5/3.75X13
- 103.554 Narrow Tapered Drill D3.75X8
- 103.555 Narrow Tapered Drill D3.75X10
- 103.556 Narrow Tapered Drill D3.75X11.5
- 103.557 Narrow Tapered Drill D3.75X13
- 105.167 Long Neo Screwdriver for Contra-angle*
- 104.060 Neo Manual Screwdriver (Medium)
- 103.558 Drill for Palatal Setter
- 125.176 Palatal Setter
- 103.395 Guided Surgery Drill 1.3

- 125.142 Fixation Clamp - 3 units per kit
- 129.034 Depth Probe
- 104.050 Torque Wrench

Note: Items that compose Neodent® Kits are sold separately.
*Check the availability.

Neodent® EasyGuide Kit for Regular/Wide Diameter Implants

Autoclavable polymer case.

The kit allows the installation of Helix GM® Implants of Ø4.0, Ø4.3 and Ø5.0 in all bone types, using the Neodent® EasyGuide Guided Surgery Technique.



Articles

- 110.314 EasyGuide Kit Reg./Wide Diam. Tray
- 125.171 GM Regular Stabilizer - 3 units per kit
- 105.163 GM Regular Driver for Contra-angle
- 105.164 GM Regular Driver for Torque Wrench
- 103.584 Regular Mucosa Punch
- 103.518 Regular Bone Leveling Drill
- 103.520 Regular Initial Drill
- 103.521 Regular Tapered Drill D2.7X8
- 103.522 Regular Tapered Drill D2.7X10
- 103.523 Regular Tapered Drill D2.7X11.5
- 103.524 Regular Tapered Drill D2.7X13
- 103.529 Regular Tapered Drill D4.0X8

- 103.530 Regular Tapered Drill D4.0X10
- 103.531 Regular Tapered Drill D4.0X11.5
- 103.532 Regular Tapered Drill D4.0X13
- 103.533 Regular Tapered Drill D4.0/4.3X8
- 103.534 Regular Tapered Drill D4.0/4.3X10
- 103.535 Regular Tapered Drill D4.0/4.3X11.5
- 103.536 Regular Tapered Drill D4.0/4.3X13
- 103.537 Regular Tapered Drill D4.3/5.0X8
- 103.538 Regular Tapered Drill D4.3/5.0X10
- 103.539 Regular Tapered Drill D4.3/5.0X11.5
- 103.540 Regular Tapered Drill D4.3/5.0X13
- 103.541 Regular Tapered Drill D5.0X8

- 103.542 Regular Tapered Drill D5.0X10
- 103.543 Regular Tapered Drill D5.0X11.5
- 103.544 Regular Tapered Drill D5.0X13
- 105.167 Long Neo Screwdriver for Contra-angle*
- 104.060 Neo Manual Screwdriver (Medium)
- 103.558 Drill for Palatal Setter
- 125.176 Palatal Setter
- 103.395 Guided Surgery Drill 1.3
- 125.142 Fixation Clamp - 3 units per kit
- 129.034 Depth Probe
- 104.050 Torque Wrench

Note: Items that compose Neodent® Kits are sold separately.
*Check the availability.

Neodent®
EasyGuide
Instruments



Narrow Tapered Drills

- :: Available in surgical steel;
- :: For Helix GM® implants with Ø3.5 and Ø3.75 in diameter;
- :: Built-in titanium stops for a fully-guided procedure, matching the color of the sleeve of the surgical guide;
- :: Color code according to implant diameter;
- :: Laser-marked length.

	Ø 3.5	Ø 3.5/3.75	Ø 3.75
8.0	103.546	103.550	103.554
10.0	103.547	103.551	103.555
11.5	103.548	103.552	103.556
13.0	103.549	103.553	103.557



Regular Tapered Drills

- :: Available in surgical steel;
- :: For Helix GM® implants with Ø4.0, Ø4.3 and Ø5.0 in diameter;
- :: Built-in titanium stops for a fully-guided procedure matching the color of the sleeve of the surgical guide;
- :: Color code according to implant diameter;
- :: Laser-marked length.

	Ø 2.7	Ø 4.0	Ø 4.0/4.3	Ø 4.3/5.0	Ø 5.0
8.0	103.521	103.529	103.533	103.537	103.541
10.0	103.522	103.530	103.534	103.538	103.542
11.5	103.523	103.531	103.535	103.539	103.543
13.0	103.524	103.532	103.536	103.540	103.544



Guided Surgery Drill 1.3 and Guide Clamp

- :: Drill available in stainless steel;
- :: Guide Clamp available in titanium;
- :: For initial fixation of the surgical guide.

Drill Ø 1.3	Guide Clamp
103.395	125.142



Drill and Palatal Setter

- :: Drill and Palatal Setter available in stainless steel;
- :: Palatal Setter placed with the GM Implant Driver for Contra-angle;
- :: Maximum torque of 20 N.cm.

Drill	Palatal Setter
103.558	125.176



Mucosa Punches

- :: Available in stainless steel;
- :: To remove the mucosa before beginning the osteotomy.
- :: Rotation recommended: 60 rpm.

Narrow	Regular
103.583	103.584



Bone Leveling Drills

- :: Available in stainless steel;
- :: Built-in titanium stops matching the color of the sleeve of the surgical guide;
- :: For flattening bone surface before osteotomy.

Narrow	Regular
103.519	103.518



Initial Drills

- :: Available in stainless steel;
- :: Built-in titanium stops matching the color of the sleeve of the surgical guide;;
- :: For rupture of the cortical bone.

Narrow	Regular
103.545	103.520



GM Drivers for Contra-Angle

- :: Available in stainless steel;
- :: Color-coded according to the sleeve of the surgical guide;
- :: To start the implant placement through the surgical guide;
- :: Maximum torque 35 N.cm.

Narrow Regular
105.161 105.163



Neo Manual Screwdriver

- :: Available in surgical steel and titanium.

Medium
25 mm

104.060



GM Drivers for Torque Wrench

- :: Available in stainless steel;
- :: To finish the implant placement through the surgical guide;
- :: Maximum torque 60 N.cm.

Narrow Regular
105.162 105.164



Neo Screwdriver Torque Connection - Contra-angle

- :: Available in stainless steel;
- :: Maximum torque 20 N.cm.

105.167



Guide Stabilizers

- :: Available in titanium;
- :: Color-coded according to the sleeve of the surgical guide;
- :: Additional fixation of the surgical guide.

Narrow Regular
125.170 125.171



Torque Wrench

- :: Available in surgical steel;
- :: Fitting for square connections;
- :: Collapsible Wrench that allows for proper assembly and cleaning.

104.050

Depth Probe

- :: Available in titanium;
- :: With marks matching the Helix GM® implant lengths.



129.034

Sleeves for Neodent® EasyGuide

- :: Available in titanium;
- :: Sold in bags with 10 units each.



125.165 Regular Sleeve D5.2



125.168 Narrow Sleeve D3.93



125.177 Sleeve for Palatal Setter



125.143 Sleeve for Fixation Clamp




A SMILE FOR EVERYONE

NEODENT® NEOARCH®

IMMEDIATE FIXED FULL-ARCH SOLUTION

Increasing expectations for shortened treatment duration represent a significant challenge for dental professionals especially in patients with anatomical deficiencies. The Neodent® Implant System offers an optimized solution for immediate fixed treatment protocols in edentulous patients even with severe atrophic maxilla. Neodent® NeoArch® allows to significantly improve patient satisfaction and quality of life by immediately restoring function and esthetics ⁽¹⁰⁾.

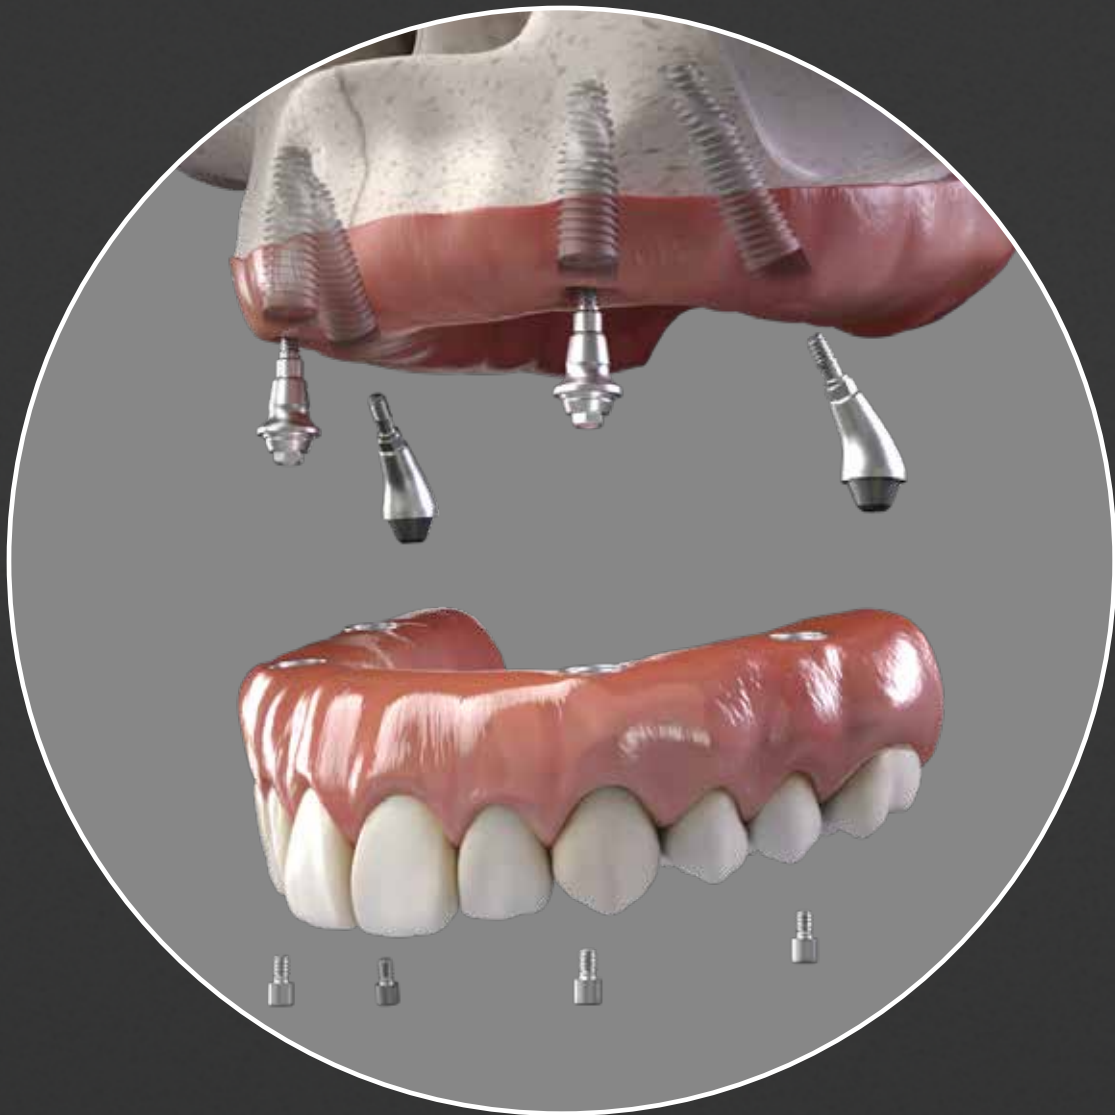

DR PEDRO RODRIGUES, from Portugal

“This amazing conical connection with these new abutments. It’s very, very nice because we can put your implants deep and you can keep that precious bone around the neck of the implant, and you put your abutment without using bone profiler, so you get the best outcome of soft tissues. //”



Immediate function resulting in shorter treatment times.

- Different implants techniques to avoid the use of grafting procedure^(1,1).
- Optimized implant design to achieve high primary stability in all bone types^(1,2).



Immediate natural-looking esthetics with versatile restorative options.

- Broad range of gingival heights to attend varied clinical needs.
- Options of straight and angled abutments (0°, 17°, 30°, 45°, 52° & 60°).



Immediate peace of mind thanks to a stable foundation.

- One connection regardless of the diameters.
- Unique connection combining Platform Switching associated with a deep 16° Morse taper including an internal indexation.

SOLUTIONS FOR ALL CLINICAL NEEDS

A implant system designed for predictable immediate treatments in all bone types even with different conditions of the residual alveolar bone.



Helix GM®



Helix GM® Long



Zygoma GM™



BONE RESORPTION



DR JOE BHAT, from United Kingdom

“NeoArch has transformed my full arch reconstructions in my practice. The amount of primary stability I guess in the GM implants is second to none. //”

Neodent® Zygoma GM™ and Helix GM® Long Implant Packaging

Neodent® packaging has been specially updated for easy handling and safe surgical procedures, providing safety from implant stocking to the capture and transport to implant bed. The implant's features, such as type, diameter and length, are identifiable on the outside of the packaging.

Three self-adhesive labels are provided for recording in the patient's medical records and for reporting to the prosthesis team. They also allows traceability for all articles.



Package instruction of use

After opening the blister, note that the implant will remain attached at the lid. In order to break the base holder of the implant, hold the lid and apply a contra-torque with the GM Connection for contra-angle (a maximum torque of 20 N.cm). Or for manual installation, use the Zygoma GM™ Implant Driver with the Neo Screwdriver Torque Connection. Finish the implant placement with the aid of the Torque Wrench.




e-IFU – Electronic Instructions For Use

Neodent® innovates once more, providing an on-line platform designed to provide quick and practical use of its own products instructions: the e-IFU (Instructions For Use) website.

To facilitate access, have the article number, which can be found on the external packaging of the product, in this catalogue or with your local distributor. Once the article number is entered in the website, the professional will have access to relevant information to this product, such as description, indication for use, contraindications, handling, traceability and other features.

Access: ifu.neodent.com.br/en

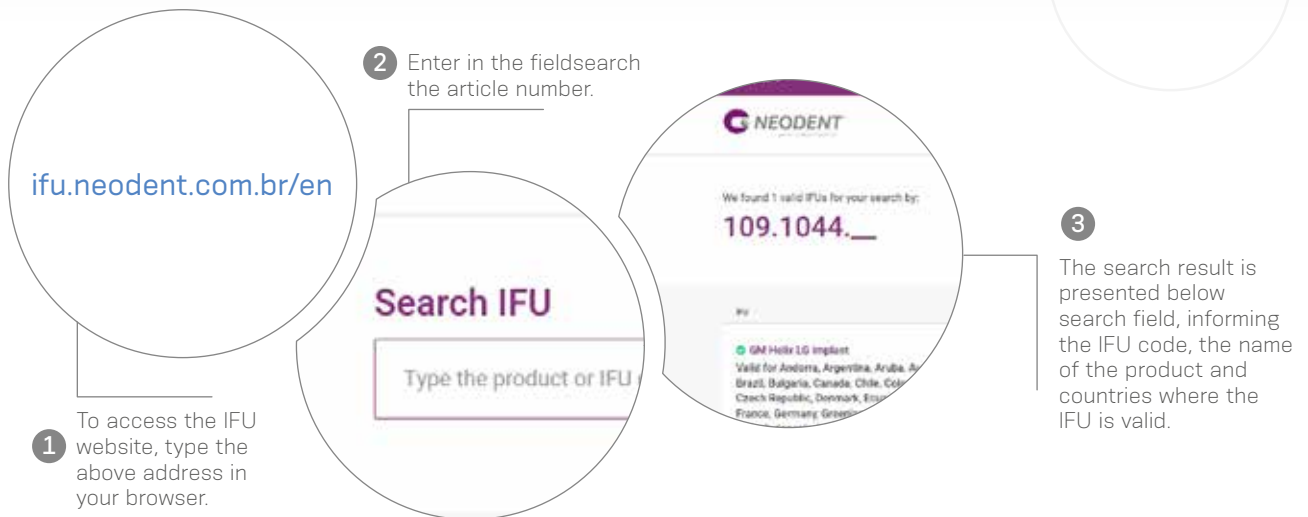

Helix GM[®] Long

PRODUCT FEATURES:

Implants Description:

- Full dual tapered implant;
- Hybrid contour with a cylindrical coronal part and conical on the apical area;
- Active apex including a soft rounded small tip and helicoidal flutes;
- Dynamic progressive thread design: from compressing trapezoidal threads on the coronal area to self-tapping threads on the apical part;
- Double lead threaded implant;
- Holder integrated to the implant body, which adapt in the packaging;
- Neoporos surface;
- Grand Morse[®] connection.

Indications:

- Indicated for surgical intraoral installation, in bone types III/IV for cases of total or partial edentulism and for multiple-unit prostheses.

Drilling features:

- For infraosseous positioning it is recommended to add 1 to 2 mm in length to the implant during surgical instrumentation.
- Drilling speed: 500-800 rpm;
- Implant insertion speed: 30 rpm;
- Maximum torque for implant placement: 60 N.cm.




Available with:

NeoPoros[®]

Drill Sequence









	Initial 103.453	Ø 2.35 103.462	Ø 3.75 103.463	Ø 4.0 103.464
Ø 3.75 mm	Optional	✓	✓	
Ø 4.0 mm	Optional	✓	✓	✓





















Bone types III and IV 

The procedure can be with Guided Surgery. Check the instruments for more information.

Helix GM® Long implants

	20.0 mm	22.5 mm	25.0 mm
Ø 3.75	 NeoPoros 109.1043	 NeoPoros 109.1044	 NeoPoros 109.1045
Ø 4.0	 NeoPoros 109.1046	 NeoPoros 109.1047	 NeoPoros 109.1048











GM Healing Abutment

	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm
Ø 3.3	 106.207	 106.208	 106.209	 106.210	 106.211	 106.212
Ø 4.5	 106.213	 106.214	 106.215	 106.216	 106.217	 106.218
Ø 5.5		 106.250	 106.251	 106.252	 106.253	
Ø 6.5		 106.254	 106.255	 106.256	 106.257	



:: Use the manual Neo Screwdriver (104.060);

:: Do not exceed the insertion torque of 10 N.cm.

GM Customizable Healing Abutments

	Profile	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm	6.5 mm
Ø 5.5	 106.223	 106.224	 106.225	 106.226	 106.227		
Ø 7.0		 106.228	 106.229	 106.230	 106.231	 106.232	

GM Cover Screw

	0 mm	2 mm
 117.021	 117.022	

:: Use the manual Neo Screwdriver (104.060);
:: Do not exceed the insertion torque of 10 N.cm.

Zygoma GM™

PRODUCT FEATURES:

Implants Description:

- Hybrid contour with a cylindrical coronal part and conical on the apical area;
- The apex has a conical profile with a spherical tip and three equally spaced helical flutes;
- Trapezoidal thread and progressive increase of the thread depth at the apical portion;
- Tissue Protect: portion without threads, near the cervical region, indexed to the hexagon face;
- Holder integrated to the implant body, which adapt in the packaging;
- Neoporos surface;
- Grand Morse® connection.

Indications:

- Indicated for surgical procedures in the the posterior region of the maxilla and in the zygoma, in cases of severe maxilla resorption. Zygomatic Implants may be used in immediate loading procedures when there is good primary stability and appropriate occlusal loading.

Drilling features:

- Drilling speed: 800-1200 rpm;
- Lateral Direction Drill speed: 600-800 rpm;
- Implant insertion speed: 30 rpm;
- Maximum torque for implant placement: 60 N.cm.

Available with:

NeoPoros®




Drill Sequence



The procedure can start guided. Check the instruments for more information.

Zygoma GM™ Implants

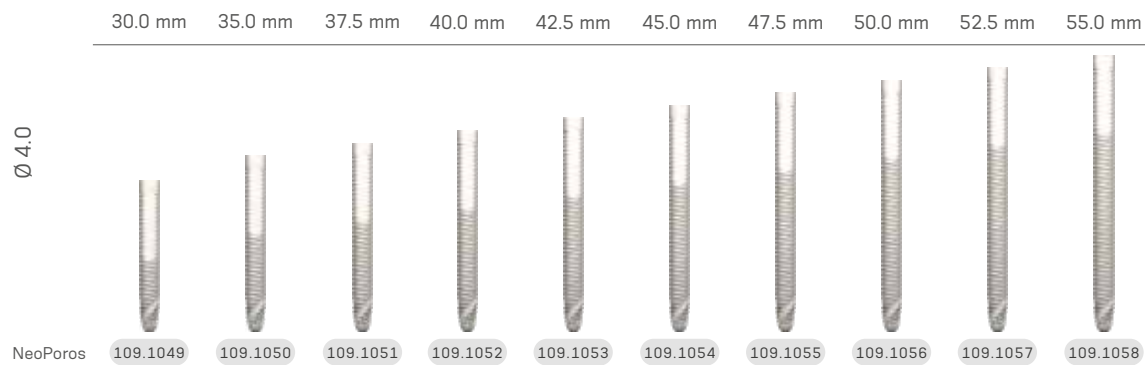

GM Cover Screw



0 mm	2 mm
117.021	117.022

- ⌘ Use the manual Neo Screwdriver (104.060);
- ⌘ Do not exceed the insertion torque of 10 N.cm.

GM Mini Conical Abutment



Multiple-unit screw-retained prosthesis



Ø 4.8 mm

Consider in addition 1.5 - 2.0 mm for the restorative material;

Minimum interocclusal space of 4.5 mm from the mucosa level for straight abutments;

Exact;

Neo Removable Screw.



Installation Sequence

1 32 N.cm
GM Mini Conical Abutment

0.8 mm	1.5 mm	2.5 mm
115.243	115.244	115.245
3.5 mm	4.5 mm	5.5 mm
115.246	115.247	115.248

OR


2 20 N.cm
GM Exact Mini Conical Abutment *
Abutment 17°/30°/45°
45°/45° slim/52°
60°

	17°	30°	45°	45° slim	52°	60°
1.5 mm	115.275	115.278	115.281	115.302	115.300	115.285
2.5 mm	115.276	115.279	115.282	115.303	115.301	115.286
3.5 mm	115.277	115.280				



Intraoral



Model Scanning



Conventional

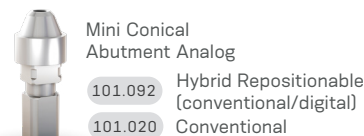



*The 45° Mini Conical Abutment, Slim, 45° Mini Conical Abutment and the 52° Mini Conical Abutment are indicated for use only with Zygoma GM™.

Drivers



Accessories

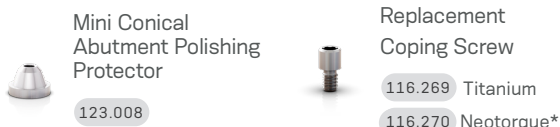

*Application of a film carbon-based coat that provides a lower friction coefficient, resulting in increased pre-load.

GM Mini Conical Abutment Coping for Removable Prosthesis



Overdenture

Recommended for overdentures in association with Mini Conical Abutments.



Installation Sequence





*The 45° Mini Conical Abutment Slim, 45° Mini Conical Abutment and the 52° Mini Conical Abutment are indicated for use only with Zygoma GM™.

*The 60° Mini Conical Abutment is indicated for use only with Zygoma GM™.


Drivers



Accessories

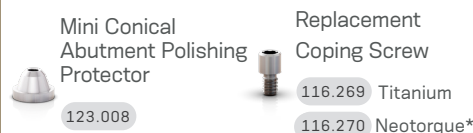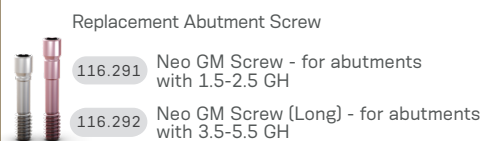


*Application of a film carbon-based coat that provides a lower friction coefficient, resulting in increased pre-load.

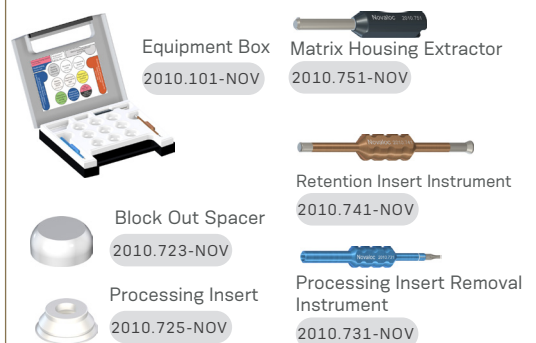


Measurements GM Mini Conical Abutment


17°

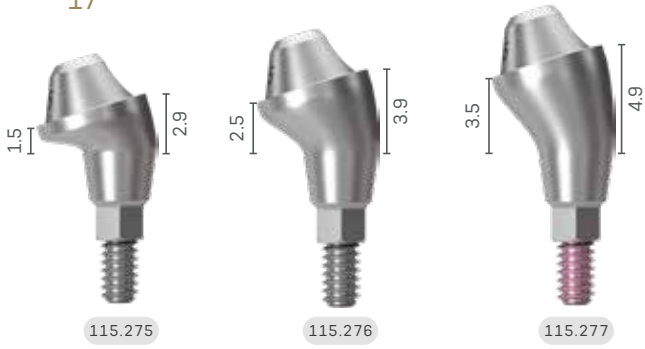


30°

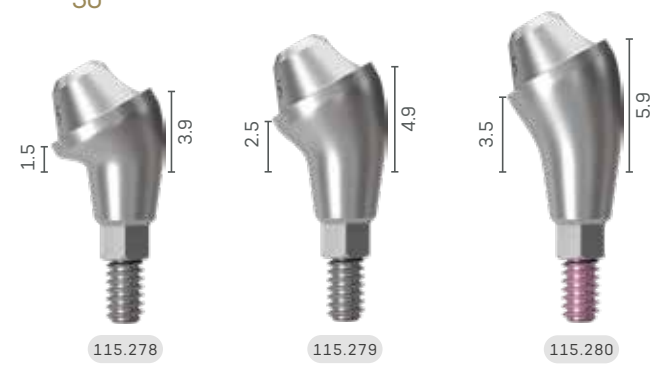

45°*

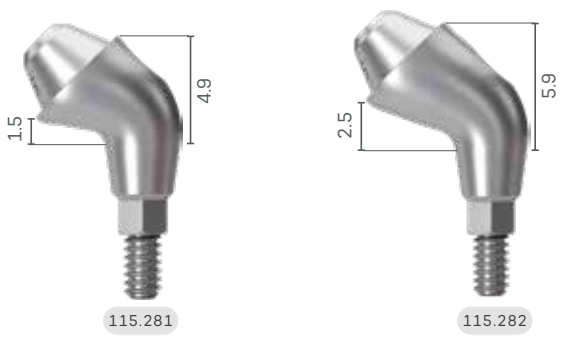

45° slim*

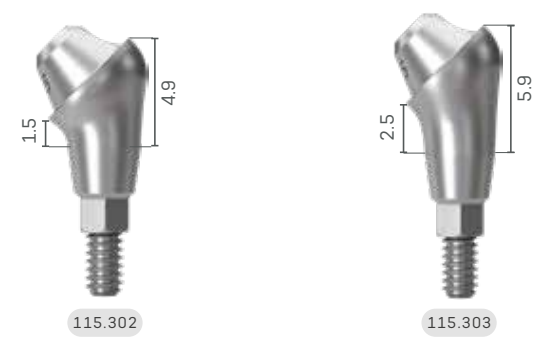

*The 45° Mini Conical Abutment is indicated for use only with Helix GM® Long and Zygoma GM™.

The 45° Mini Conical Abutment Slim is indicated for use only with Zygoma GM™.

52°*



60°*




The 52° Mini Conical Abutment is indicated for use only with Zygoma GM™.

*The 60° Mini Conical Abutment is indicated for use only with Zygoma GM™.

NeoArch[®] Kits

Helix GM® Long Compact Surgical Kit

Autoclavable polymer case.

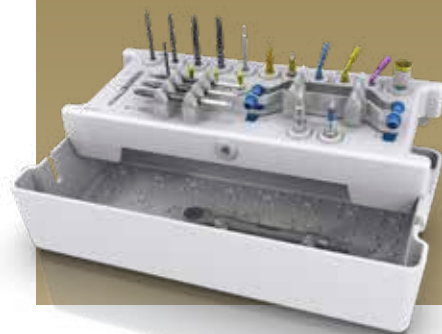

Articles

110.300 Helix GM® Long Compact Surgical Kit Case

103.395 Guided Surgery Drill 1.3mm

125.100 Guided Surgery Guide Clamp

125.140 Drill Guide For NGS Helix GM® Long 2.0/2.35mm

125.141 Drill Guide For NGS Helix GM® Long 3.75/4.0mm

103.459 Twist Drill For NGS Helix GM® Long 2.35mm

103.460 Twist Drill For NGS Helix GM® Long 3.75mm

103.461 Twist Drill For NGS Helix GM® Long 4.0mm

103.453 Helix GM® Long Initial Drill 2.0mm

103.462 Twist Drill For Helix GM® Long 2.35mm

103.463 Twist Drill For Helix GM® Long 3.75mm

103.464 Twist Drill For Helix GM® Long 4.0mm

129.021 Helix GM® Long X-ray Positioner

128.032 GM Angle Measurer 17°

128.033 GM Angle Measurer 30°

128.034 GM Angle Measurer 45°

105.143 Regular Guided Surgery GM Connection for Torque Wrench

105.140 Regular Guided Surgery GM Connection - Contra-angle

104.060 Neo Manual Screwdriver (medium)

105.129 GM Implant Driver - Torque Wrench (short)

105.131 GM Implant Driver - Contra-angle

104.050 Torque Wrench

Note: Items that compose Neodent® Kits are sold separately.

Zygoma GM™ Surgical Kit

Autoclavable polymer case.



Articles

110.299 Zygoma GM™ Surgical Kit Case

103.395 Guided Surgery Drill 1.3mm

125.100 Guided Surgery Guide Clamp

125.139 Drill Guide For Ngs Zygoma GM™ 2.35mm

103.454 Twist Drill For Ngs Zygoma GM™ 2.35mm

103.455 Twist Drill For Zygoma GM™ 2.35mm

103.456 Twist Drill For Zygoma GM™ 3.75mm

103.457 Twist Drill For Zygoma GM™ 4.0mm

103.458 Lateral Direction Drill For Zygoma GM™ 4.0mm

103.465 Pilot Twist Drill For Zygoma GM™ 2.3/3.2mm

104.063 Zygoma GM™ Installation Driver

129.022 Zygoma GM™ Probe 2.35mm

129.023 Zygoma GM™ Probe 4.0mm

128.032 GM Angle Measurer 17°

128.033 GM Angle Measurer 30°

128.034 GM Angle Measurer 45°

128.028 GM Height Measurer

104.060 Neo Manual Screwdriver (medium)

105.129 GM Implant Driver - Torque Wrench (short)

105.131 GM Implant Driver - Contra-angle

104.050 Torque Wrench

Note: Items that compose Neodent® Kits are sold separately.

NeoArch[®] Instruments



Helix GM® Long Drills

- :: Available in surgical steel;
- :: Drill sequence for Helix GM® Long implants.

Initial	Ø 2.35	Ø 3.75	Ø 4.0
103.453	103.462	103.463	103.464



Helix GM® Long Drills for Guided Surgery

- :: Available in surgical steel;
- :: Drill sequence for Helix GM® Long implants on Guided Surgery.

Ø 2.35	Ø 3.75	Ø 4.0
103.459	103.460	103.461



Zygoma GM™ Drills

- :: Available in surgical steel;
- :: Drill sequence for Zygoma GM™ implants.

	Pilot			
Ø 2.35	Ø 2.3/3.2	Ø 3.75	Ø 4.0	
103.455	103.465	103.456	103.457	



Zygoma GM™ Lateral Direction Drill

- :: Available in surgical steel;
- :: Spherical tip with guide pin and helical blades for preparing the site for the implant placement in the exteriorized technique.


Ø 4.0
103.458



Zygoma GM™ Drill for Guided Surgery

- :: Available in surgical steel;
- :: After using the first drill, the surgical guide must be removed and the conventional protocol must be started.

Ø 2.35
103.454



GM Height Measurer

- :: Available in titanium;
- :: For selecting GM prosthetic abutments;
- :: Marks corresponding to transmucosa heights.
- :: Can be used as X-Ray Positioner.

128.028



GM Implant Driver - Contra-Angle

- :: To capture the implant directly from the packaging;
- :: To place GM Implants with contra-angle, or attached to a manual driver for contra-angle connections (104.028) for hand placement;
- :: With six dimples to indicate the hex index face position;
- :: The laser marks indicate the depth of implant placement, bone level, 1 and 2mm infra-bone and last marking (3mm) biological space;
- :: Maximum torque 35 N.cm.

105.131



GM Implant Driver - Torque Wrench

- :: To place GM Implants with the Torque Wrench (104.050);
- :: With six marks to indicate the hex index face position;
- :: The laser marks indicate the depth of implant placement, bone level, 1 and 2mm infra-bone and last marking (3mm) biological space;
- :: Maximum torque: 60 N.cm.

Short	Long	Extra-long
22 mm	30 mm	45 mm
105.129	105.130	105.156



Neo Screwdriver Torque Connection - Torque Wrench

- :: Available in surgical steel;
- :: Yellow color for line identification.

Short	Medium	Long
16.5 mm	22 mm	32 mm
105.133	105.132	105.157



Neo Manual Screwdriver

- :: Available in surgical steel;
- :: Yellow color for line identification.

Short	Medium	Long
21 mm	25 mm	37 mm
104.058	104.060	104.070

Neo Screwdriver Torque Connection - Contra-angle



:: Available in surgical steel;
 :: Yellow color for line identification;
 :: Medium Neo Screwdriver Torque Connection
 :: Extra Short Neo Screwdriver Torque Connection - Contra-angle (105.146) recommended for Impression Copings, Cover Screws and Healing Abutments.

Extra Short	Short	Long
16.5 mm	24 mm	37 mm
105.146	105.135	105.167

Hexagonal Prosthetic Driver



:: Available in surgical steel;
 :: To install and apply torque over straight GM Mini Conical Abutments and GM Micro Abutments;
 :: Yellow color for line identification.

Contra-angle	Torque Wrench
105.138	105.137

GM Bone Profile Drill with Guide



:: Available in surgical steel;
 :: Used in the surgical second step;
 :: Conforms the bone around the implant platform, preparing the emergence profile to be suitable to prosthetic components.

103.424

GM Angle Measurer



:: Available in titanium;
 :: To a more accurate selection and planning of the abutments angulation during the prosthetic phase.

17°	30°	45°	52°	60°
128.032	128.033	128.034	128.043	128.035

Helix GM® Long Drill Guide for Guided Surgery



:: Instrument with the purpose of guiding the drills during the bone bed preparation according to the guided surgery technique.

Ø 2.0/2.35	Ø 3.75/4.0
125.140	125.141

Zygoma GM™ Drill Guide for Guided Surgery



:: Instrument with the purpose of starting the Zygomatic Surgery guided.

Ø 2.35
125.139

Guided Surgery Drill 1.3 and Guide Clamp



:: Drill available in surgical steel;
 :: Guide Clamp available in titanium;
 :: For initial fixation of the surgical guide.

Drill Ø 1.3	Guide Clamp
103.395	125.100

Guided Surgery GM Connection - Contra-Angle



:: Available in stainless steel;
 :: To start the implant placement through the surgical guide.

Regular
 105.140

Guided Surgery GM Connection - Torque Wrench



:: Available in stainless steel;
 :: To finish the implant placement through the surgical guide.

Regular
 105.143

Helix GM® Long X-ray Positioner



:: Indicated for evaluation of the osteotomy depth in the implant placement procedure.

129.021

Zygoma GM™ Probes



:: Available in Stainless Steel;
 :: The probe for the drill Ø2.35 mm has a tip design in L;
 :: The probes for the drills Ø3.5 and Ø3.75 mm have a tip with a design similar to the apex of the correspondent drill that allows identifying the correct drilling depth for implant anchorage.

Ø 2.35	Ø 4.0
129.022	129.023

Zygoma GM™ Installation Driver



:: Instrument for application of manual torque.

104.063



Torque Wrench

- :: Available in surgical steel;
- :: Fitting for square connections;
- :: Collapsible Wrench that allows for proper assembly cleaning;
- :: For full instructions see page 80.

104.050



Remover for Abutments with internal threads

- :: Available in surgical steel;
- :: To remove abutments with internal threads from the implants, after removal of the screws;
- :: Compatible with abutments with Neo removable Screws

130.118 Long
130.114



Remover for Neo Screws

- :: Available in surgical steel;
- :: Compatible with Neo removable screws for abutments

130.119 Long
130.115

Removal Sets for Abutments with internal threads and Neo Screws

- :: Available in surgical steel;
- :: To remove Neo Removable Screws and abutments with internal threads from the implants, after removal of the screws;
- :: Compatible with abutments with Neo removable Screws



130.117

Long
130.116

GRAND MORSE® NEODENT® GUIDED SURGERY.

GRAND POSSIBILITIES WITH A LIMITLESS SOLUTION

Patients' expectations regarding tooth replacement are increasing and are even higher when it comes to treatment duration and esthetic outcomes. The Neodent® Guided Surgery helps clinicians to provide prosthodontically driven treatments, enabling them to perform immediate protocols with peace of mind, fulfilling patients' expectations.



DR IVA MILINKOVICH, from Serbia

“What I like about the system is implant designed, the selection of surgical components, and the possibilities of using it in guided surgery. I find it really user-friendly and the wide selection of implants and diameters.”

DIFFERENTIATE YOUR PRACTICE WITH GUIDED SURGERY.



Improve patient quality of life.

- Functional with an immediate fixed restoration.
- Esthetical with a personalized restoration and less bone remodeling ⁽¹³⁾.
- Comfort by the reduction of operative and postoperative discomfort (e.g. reduced patient chair time).



Access to more treatment options.

- Reliable access to flapless surgery ⁽¹⁴⁻¹⁶⁾.
- Designed to reduce bone grafting procedures.
- Predictable immediate protocols.



Increase patient acceptance.

- Better communication building trust with patients.
- Reliable treatment estimates from root to tooth including components and procedures.

SURGICAL PREDICTABILITY AND EFFICIENCY WITH A LIMITLESS SOLUTION.

Guided surgery is designed to reduce chair time and postoperative discomfort. It helps increasing implant positioning accuracy ⁽¹⁷⁾.



Complete
Helix® and Drive GM®
Implants portfolio




Convenient
Color-coded instruments
and symbol-marked



Flexible
2 sleeve height positions



Guided implant
insertion



Guided bed
preparation

Neodent® Guided Surgery Kit for Grand Morse®


Compatible with major guided
surgery software



Neodent[®] Guided Surgery Kit

Grand Morse® Guided Surgery Surgical Kit

Autoclavable polymer case.
The Kit allows the use of Helix GM® and Drive GM® Implants in the Guided Surgery technique.

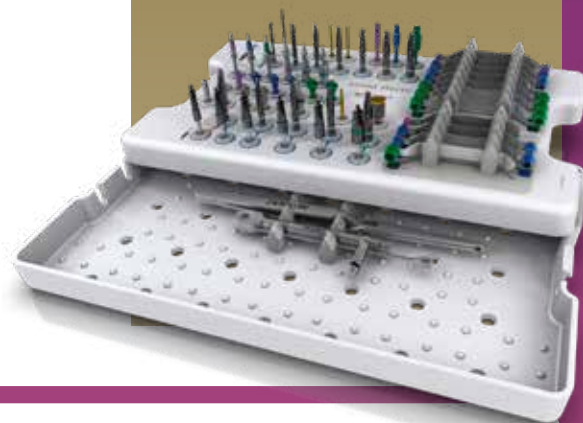

Articles

- | | | | |
|---------|---|---------|---|
| 110.296 | GM Guided Surgery Surgical Kit Case | 104.060 | Neo Manual Screwdriver (Medium) |
| 103.395 | Guided Surgery 1.3 | 103.439 | Tapered Contour Guided Surgery Drill 3.5* |
| 125.100 | Guided Surgery Guide Clamp | 103.440 | Tapered Contour Guided Surgery Drill 3.75* |
| 103.429 | Narrow Guided Surgery Punch - Contra-Angle | 103.441 | Tapered Contour Guided Surgery Drill 4.0* |
| 103.430 | Regular Guided Surgery Punch - Contra-Angle | 103.442 | Tapered Contour Guided Surgery Drill 4.3* |
| 103.431 | Wide Guided Surgery Punch - Contra-Angle | 103.443 | Tapered Contour Guided Surgery Drill 5.0* |
| 103.432 | Guided Surgery Drill 2.0 | 103.444 | Narrow Guided Surgery GM Pilot Drill 3.5 |
| 103.433 | Tapered Guided Surgery Drill 3.5* | 103.445 | Regular Guided Surgery GM Pilot Drill 3.5 |
| 103.434 | Tapered Guided Surgery Drill 3.75* | 103.446 | Guided Surgery GM Pilot Drill 3.75 |
| 103.435 | Tapered Guided Surgery Drill 4.0* | 103.447 | Guided Surgery GM Pilot Drill 4.0 |
| 103.436 | Tapered Guided Surgery Drill 4.3* | 103.448 | Guided Surgery GM Pilot Drill 4.3 |
| 103.437 | Tapered Guided Surgery Drill 5.0* | 103.449 | Guided Surgery GM Pilot Drill 5.0 |
| 103.438 | Tapered Guided Surgery Drill 6.0* | 125.119 | Narrow Guided Surgery Drill Guide 2.0/3.5 |
| 105.139 | Narrow Guided Surgery GM Connection - Contra-angle | 125.121 | Regular Guided Surgery Drill Guide 2.0/3.5 |
| 105.140 | Regular Guided Surgery GM Connection - Contra-angle | 125.122 | Regular Guided Surgery Drill Guide 3.75/4.0 |
| 105.141 | Wide Guided Surgery GM Connection - Contra-angle | 125.123 | Regular Guided Surgery Drill Guide 4.3 |
| 105.142 | Narrow Guided Surgery GM Connection for Torque Wrench | 125.126 | Wide Guided Surgery Drill Guide 2.0/3.5 |
| 105.143 | Regular Guided Surgery GM Connection for Torque Wrench | 125.127 | Wide Guided Surgery Drill Guide 4.0/4.3 |
| 105.144 | Wide Guided Surgery GM Connection for Torque Wrench | 125.128 | Wide Guided Surgery Drill Guide 5.0/6.0 |
| 125.130 | Narrow Guided Surgery GM Guide Stabilizer | 125.120 | Narrow Tapered Contour Guided Surgery Drill Guide 3.5 |
| 125.131 | Regular Guided Surgery GM Guide Stabilizer | 125.124 | Regular Tapered Contour Guided Surgery Drill Guide 3.5/3.75 |
| 125.132 | Wide Guided Surgery GM Guide Stabilizer | 125.125 | Regular Tapered Contour Guided Surgery Drill Guide 4.0/4.3 |
| 125.133 | Narrow Guided Surgery GM Guide Stabilizer (Long) | 125.129 | Wide Tapered Contour Guided Surgery Drill Guide 5.0 |
| 125.134 | Regular Guided Surgery GM Guide Stabilizer (Long) | 129.001 | Titanium Tweezers |
| 105.145 | Guided Surgery GM H11 Connection for Torque Wrench | 104.050 | Torque Wrench |
| 105.136 | Neo Screwdriver Torque Connection - Contra-angle (Medium) | | |

Note: Items that compose Neodent® Kits are sold separately.

*Conventional guided surgery drills that can be replaced by the respective short version.

Neodent®
Guided Surgery
Instruments



Guided Surgery Tapered Drills

- :: Available in surgical steel;
- :: Drill sequence for Helix GM® and Drive GM® Implants in the guided surgery technique;
- :: Fully guided technique with Short Drills indicated for 8, 10 or 11.5 mm long implants.

	Ø 2.0	Ø 3.5	Ø 3.75	Ø 4.0	Ø 4.3	Ø 5.0	Ø 6.0
Short 36.5 mm	103.475	103.476	103.477	103.478	103.479	103.480	103.481
Regular 41 mm	103.432	103.433	103.434	103.435	103.436	103.437	103.438



Guided Surgery Tapered Contour Drills

- :: Available in surgical steel;
- :: Drill sequence for Helix GM® Implants in the guided surgery technique for bone types I or II;
- :: Fully guided technique with Short Drills indicated for 8, 10 or 11.5 mm long implants.

	Ø 3.5+	Ø 3.75+	Ø 4.0+	Ø 4.3+	Ø 5.0+
Short 36.5 mm	103.482	103.483	103.484	103.485	103.486
Regular 41 mm	103.439	103.440	103.441	103.442	103.443



Guided Surgery GM Pilot Drills

- :: Available in surgical steel;
- :: Color-coded according to the sleeve diameter;
- :: Recommended for Helix GM® in bone types I or II;
- :: Optional Drive GM® in bone types III or IV.

	Narrow	Regular	Wide
Ø 3.5	103.444	Ø 3.5 103.445	Ø 5.0 103.449
		Ø 3.75 103.446	
		Ø 4.0 103.447	
		Ø 4.3 103.448	



Guided Surgery Drill 1.3 and Guide Clamp

- :: Drill available in surgical steel;
- :: Guide Clamp available in titanium;
- :: For initial fixation of the surgical guide.

Drill Ø 1.3	Guide Clamp
103.395	125.100



Guided Surgery Punch - Contra-Angle

- :: Available in titanium;
- :: Color-coded according to the sleeve diameter;
- :: To remove the mucosa before beginning the osteotomy.

Narrow	Regular	Wide
103.429	103.430	103.431



Guided Surgery Drill Guides

- :: Available in titanium and stainless steel;
- :: Color-coded according to the sleeve diameter;
- :: To fit in the sleeve in the surgical guide;
- :: To be used with correspondent drill diameter and type.

	Narrow	Regular	Wide
Ø 2.0/3.5	125.119	Ø 2.0/3.5 125.121	Ø 2.0/3.5 125.126
Ø 3.5+	125.120	Ø 3.75/4.0 125.122	Ø 4.0/4.3 125.127
		Ø 4.3 125.123	Ø 5.0/6.0 125.128
		Ø 3.5+/3.75+ 125.124	Ø 5.0+ 125.129
		Ø 4.0+/4.3+ 125.125	



Guided Surgery GM Connection - Contra-Angle

- :: Available in stainless steel;
- :: Color-coded according to the sleeve diameter;
- :: To start the implant placement through the surgical guide.

Narrow Regular Wide
 105.139 105.140 105.141



Guided Surgery Guide Stabilizers

- :: Available in titanium;
- :: Color-coded according to the sleeve diameter;
- :: Additional fixation of the surgical guide.

Narrow Regular Wide
 125.130 125.131 125.132



Guided Surgery GM Connection - Torque Wrench

- :: Available in stainless steel;
- :: Color-coded according to the sleeve diameter;
- :: To finish the implant placement through the surgical guide.

Narrow Regular Wide
 105.142 105.143 105.144



Guided Surgery Guide Stabilizers - Long

- :: Available in titanium;
- :: Additional fixation of the surgical guide;
- :: To be used when the H11 sleeve height is chosen.

Narrow Regular
 125.133 125.134



Guided Surgery GM H 11 Connection - Torque Wrench

- :: Available in stainless steel;
- :: To finish the implant placement through the surgical guide;
- :: To be used when the H11 sleeve height is chosen.

105.145

Sleeves for Neodent® Guided Surgery System

- :: Available in titanium;
- :: Sold in bags with 10 units each.



- 125.135 Sleeve for Narrow Guided Surgery System
- 125.136 Sleeve for Regular Guided Surgery System
- 125.137 Sleeve for Wide Guided Surgery System
- 125.138 Sleeve of Setter for Guided Surgery System

Neodent® Helix GM Narrow

SMALL DIAMETER, GREAT ACHIEVEMENTS.

Bring reliability to your practice through the next generation of immediate esthetic solutions for reduced interdental spaces and bone availability.

The Ø 2.9mm Helix GM Narrow provides an immediate, small diameter solution seeks to provide simplicity for treatment protocol – regardless of whether guided or non-guided techniques are used – confidence without compromising on strength, and flexibility for immediate esthetic outcomes in limited interdental spaces.

Ø 2.9



CONFIDENCE WITH A STABLE LONG-TERM IMPLANT FOUNDATION


Implant therapy for demanding indications, such as reduced interdental spaces, can raise concerns regarding resistance and biomechanical behavior. Therefore, features of an implant-abutment interface are essential to provide successful long-term functional, stable, and esthetic results.

The Ø 2.9mm Helix features the strong and stable GM Narrow connection, designed with a unique combination based on proven concepts seeking to achieve long lasting results. A system produced out with the commercially pure titanium grade 4 offering treatment predictability through the Acqua hydrophilic surface.

RELIABLE AND STRONG GM NARROW CONNECTION


16° Morse Taper connection

The implant-abutment interface is a relevant aspect that could interfere on the success of patient's outcome. Helix GM Narrow is designed to deliver a tight fit for optimal connection sealing and offers strong mechanical resistance.



Internal hexagonal indexation

The connection is designed with internal hexagonal indexation for precise abutment positioning, easy handling.




Platform switching

The abutment design features a narrower diameter than the implant coronal area, which enables platform switching. ⁽⁵⁻⁹⁾



Screw-retained interface

The Helix GM Narrow features a morse taper screw-retained connection, which fits into the internal thread with precision seeking to provide a stable abutment connection.



COMMERCIALLY PURE AND MECHANICALLY STRONG TITANIUM GRADE 4

Beyond a versatile design allowing primary stability, the Helix GM Narrow is produced from the most commercially pure and mechanically strong titanium grade 4 (Ti Gr 4). Static torsion tests have been conducted providing a greater performance and strongness of +12,7% than the former small diameter Neodent® system (Ti6Al4V-ELI).

Static torsion test

+ 12,7%

New small diameter Neodent® system (Ti Gr 4)

Former small diameter Neodent® system (Ti6Al4V-ELI)

Font: Annex_NoC Helix Narrow internal document.



ACQUA HYDROPHILIC SURFACE'S AND TREATMENT PREDICTABILITY

The Neodent® Acqua hydrophilic surface is the next level of the highly successful S.L.A. surface. It was developed to reach expected results outcomes even in the most challenging patient cases, such as soft bone or immediate protocols. ⁽¹⁻⁴⁾



SIMPLICITY FOR TREATMENT PROTOCOLS

The Helix GM Narrow system provides an intuitive hybrid surgical kit designed to best suit any chosen surgical procedure, whether conventional or guided, adding even more simplicity to the system by using the Neo Screw connection.

An intuitive and functional compact surgical cassette

The Helix GM Narrow system allows intuitive conventional and guided surgeries with the functional compact surgical kit, to support improve outcomes and patient satisfaction.

A predictable guided procedure with the easyguide concept

The Neodent® EasyGuide concept offers straightforward guided surgery technique enabling surgical convenience with one-hand procedures, and pursuing predictable surgical results with confidence for accurate implant positioning.

One Screwdriver available both for Neodent® GM and GM Narrow

The Helix GM Narrow system features the Neo Screwdriver, which has a star attachment offering reliability and durability, compatible with all GM Narrow healing abutments and restorative screws.





FLEXIBILITY FOR IMMEDIATE ESTHETIC OUTCOMES


Patients lacking bone availability in the esthetic zone or experiencing limited space between adjacent teeth, can make tooth replacement procedures challenging for implant clinicians. When coupled with a lack of adequate prosthetic options to correctly replace missing teeth, patient satisfaction declines, and practices can suffer.

The versatile Neodent® Helix GM Narrow system combines a Ø2.9mm Helix implant, with a comprehensive prosthetic portfolio to restore cases in limited bone availability and interdental spaces, for immediate esthetic results.


THE UNBEATABLE VERSATILITY OF HELIX

Dynamic progressive thread design


- Coronal: Double start threads with rounded root > compressing;
- Apex: V-Shape > Self-cutting High primary stability.



- #### Tapered body design
- Coronal: Progressive tapered design;
 - Apex: 12° Under-osteotomy for bone types 3 and 4.



- #### Hybrid contour
- Coronal: Cylindrical;
 - Apex: Conical.



- #### Active Apex
- Short tip;
 - Helicoidal flutes.



DR FEDERICO MANDELLI, from Italy

“I think that today an implant system should be very flexible and we don't have to change implants based on our clinical needs. That's why I decided to choose the Neodent® product, because with just one implant I can perform any kind of treatment. //”



**A SOLUTION FOR LIMITED BONE AVAILABILITY
IN ALL BONE TYPES**

Indicated for all bone types, the Neodent® Helix GM Narrow is specifically engineered to address esthetic challenges in situations with limited bone, thanks to its small diameter implant of 2.9mm.



**COMPREHENSIVE PROSTHETIC PORTFOLIO FOR OPTIMIZED
ESTHETIC AND FUNCTIONAL RESULTS**

The Helix GM Narrow system was designed to offer clinicians greater levels of treatment flexibility with a comprehensive prosthetic portfolio, designed to meet patient expectations regarding short treatment times, esthetic and functional results.

It allows single and multi-unit restorations from screw and cement-retained, to removable prosthesis. The system also allows support for conventional and digital workflows supporting provide natural-looking restorations using either conventional or immediate protocols.



Titanium
Temporary Abutment



Titanium
Base



Universal
Abutment



Micro
Abutment



Attachment
Removable



Single-unit screw-
retained prosthesis



Single-unit cement-
retained prosthesis



Multiple-unit screw-
retained prosthesis



Temporary



Overdenture

Neodent® Helix GM Narrow Implant Packaging

Neodent® packaging has been specially updated for easy handling and seeking to achieve a safe surgical procedure, providing practicality from implant stocking to the capture and transport and implant bed. The implant's features, such as type, diameter and length, are readily identifiable on the outside of the packaging.

Three self-adhesive labels are provided for recording in the patient's medical records and for reporting to the prosthesis team. They also allow traceability for all articles.



Package instruction of use



1. The cardboard and blister packagings must be opened, manually, without the use of sterile gloves. Break the seal of the cardboard packaging and remove the blister. Open the blister pack. Deposit the sterile flask over the surgical field.

Note: the clear tube and implant must be handled with a sterile surgical glove, in a surgical environment. Hold the bottle using the non-dominant hand and take the lid off.



2. Hold the bottle using the non-dominant hand and take the lid off. The internal support containing the implant should come out attached to the lid. To do so, remove the lid and the clear tube's internal support in the axial direction making no lateral movements.



3. Using the non-dominant hand, press the sides of the internal support promoting a "pincer effect" and immobilizing the implant. Keep the support pressed and remove the lid.



4. For installation, hold the implant with the driver for contra angle, keeping the connection stable and slightly rotating the internal support, searching for the perfect fit between the connection and the implant.



5. Take the implant to the surgical cavity.





6. Place the implant to its final position with a maximum torque of 35 N.cm and speed of 30 rpm, clockwise.

e-IFU – Electronic Instructions For Use

Neodent® innovates once more, providing an on-line platform designed to provide quick and practical use of its own products instructions: the e-IFU (Instructions For Use) website.

To facilitate access, have the article number, which can be found on the external packaging of the product, in this catalogue or with your local distributor. Once the article number is entered in the website, the professional will have access to relevant information to this product, such as description, indication for use, contraindications, handling, traceability and other features.

Access: ifu.neodent.com.br/en

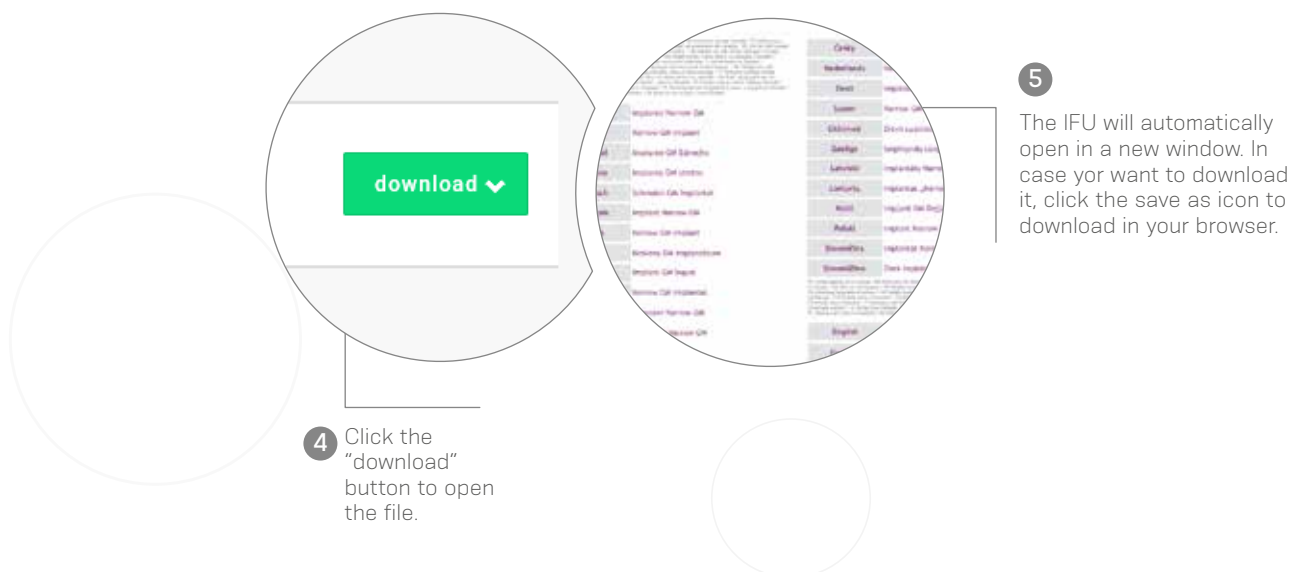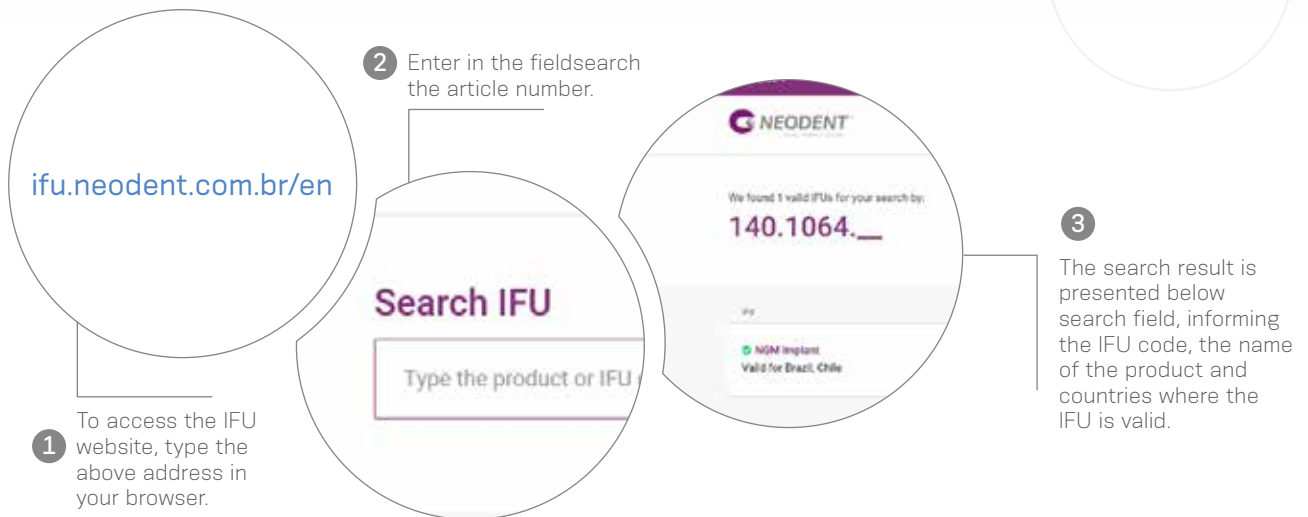

Helix GM Narrow

PRODUCT FEATURES:

Implants Description:

- Progressive tapered design;
- Hybrid contour with a cylindrical coronal part and conical on the apical area;
- Active apex with rounded short tip and helicoidal flutes; 12° under-osteotomy for bone types 3 and 4;
- Dynamic progressive thread design: from compressing trapezoidal threads on the coronal area to self-cutting V-shape threads on the apical part;
- Double threaded implant;
- GM Narrow connection.

Indications:

- Indicated for all types of bone density in the region of lateral incisors in the maxilla or in the region of lateral and central incisors in the mandible.

Drilling features:

- NGM Countersink Drill is required in bone types I and II;
- Implant should be positioned 2 mm below bone level;
- Drilling speed: 800-1200 rpm for bone type I and II;
- Drilling speed: 500-800 rpm for bone type III and IV;
- Implant insertion speed: 30 rpm;
- Maximum torque for implant placement: 35 N.cm.

Available with:

acqua®



Drill Sequence for conventional surgery



10 mm	✓	✓			✓			✓
12 mm	✓		✓			✓		✓
14 mm	✓			✓			✓	✓

*Optional / Bone types I and II

10 mm	✓	✓*						
12 mm	✓		✓*					
14 mm	✓			✓*				

*Optional / Bone types III and IV

Drill Sequence for guided surgery



10 mm	✓*	✓*	✓	✓			✓		✓
12 mm	✓*	✓*	✓		✓			✓	✓
14 mm	✓*	✓*	✓			✓		✓	✓

*Optional / Bone types I and II


10 mm	✓*	✓*	✓	✓*					
12 mm	✓*	✓*	✓		✓*				
14 mm	✓*	✓*	✓			✓*			

*Optional / Bone type III


10 mm									
12 mm	✓*	✓*	✓						
14 mm	✓*	✓*	✓						

*Optional / Bone type IV


Helix GM Narrow Implants

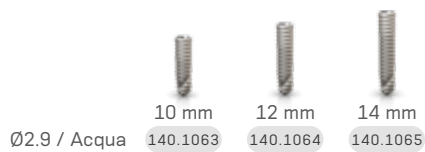

NGM Cover Screw



NGM Healing Abutment

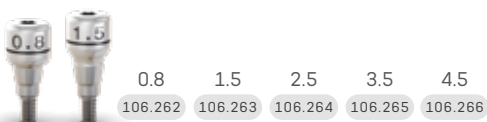

NGM Micro Abutment



Single-unit screw-retained prosthesis



Multiple-unit screw-retained prosthesis



Ø 3.5 mm

Gingival heights:
0.8, 1.5, 2.5 & 3.5 mm.



Recommended for anterior region.

Installation Sequence

0.8 mm	1.5 mm	NGM Micro Abutment
115.287	115.288	
2.5 mm	3.5 mm	
115.289	115.290	




Intraoral



Model Scanning



Conventional

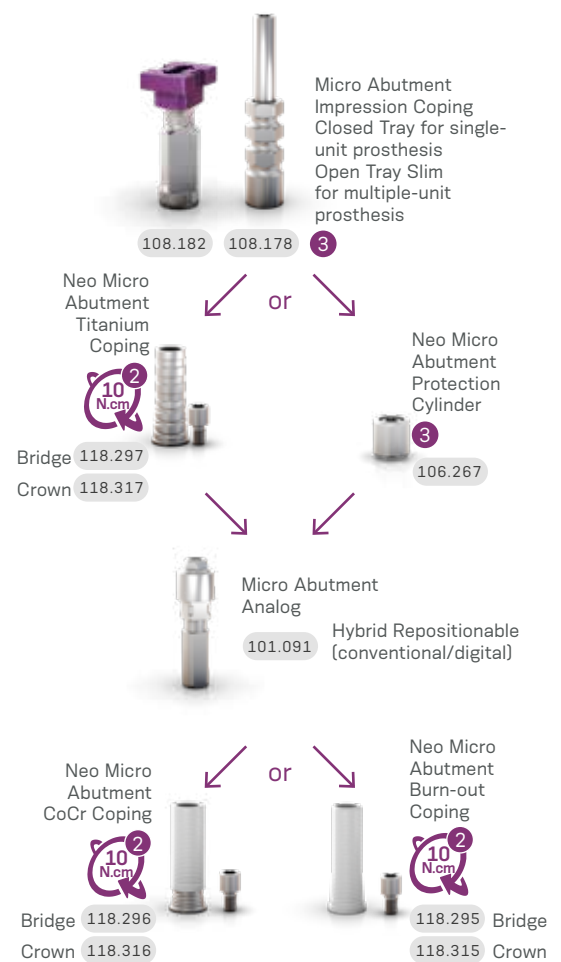

Drivers

- Hexagonal Prosthetic Driver + Torque Wrench
- Neo Screwdriver Torque Connection + Torque Wrench
- Neo Screwdriver Torque Connection + Manual Screwdriver Torque

Accessories

- Micro Abutment Polishing Protector (123.015) Bridge
- Replacement Coping Screw (116.269) Titanium (116.270) Neotorque*

*Application of a film carbon-based coat that provides a lower friction coefficient, resulting in increased pre-load.

NGM Universal Abutment



Single-unit
cement-retained
prosthesis



Ø 3.3 mm

Cementable area: 4.0 or 6.0 mm;

Click retention for
provisional copings;

Exact;

Neo Removable screw;



Installation Sequence



NGM Exact Click
Universal Abutment

	0.8 mm	1.5 mm	2.5 mm	3.5 mm
4 mm	114.902	114.903	114.904	114.905
6 mm	114.906	114.907	114.908	114.909

or



NGM Exact Click
Universal Abutment 17°

	1.5 mm	2.5 mm	3.5 mm
4 mm	114.910	114.911	114.912
6 mm	114.913	114.914	114.915

Intraoral



Universal Abutment
Intraoral Scanbody

4 mm	6 mm	Ø 3.3
108.143	108.144	



Universal abutment Hybrid
Repositionable analog

4 mm	6 mm	Ø 3.3
101.097	101.098	

Milled crown

Conventional



Click Universal
Abutment
Impression Coping

4 mm	6 mm	Ø 3.3
108.172	108.173	

Click Universal
Abutment
Provisional Coping



4 mm	6 mm	Ø 3.3
118.304	118.305	

Universal Abutment
Hybrid Repositionable
Analog



4 mm	6 mm	Ø 3.3
101.097	101.098	

Universal Abutment
Burn-out Coping



4 mm	6 mm	Ø 3.3
118.181	118.182	

Drivers

1



Neo
Screwdriver
Torque
Connection

+



Torque Wrench

Accessories



Replacement
Sterile Screws

116.294 Titanium

116.293 Neotorque*

NGM Titanium Base



Single-unit screw-retained prosthesis



Single-unit cement-retained prosthesis



Ø 3.5 mm

- Customizable up to 4 mm high;
- Cementable area: 6.0 or 4.0 mm;
- Exact;
- Neo Removable screw;




Installation Sequence

Intraoral



Model Scanning

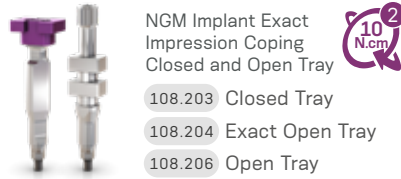


NGM Exact Titanium Base for Crown Ø 3.5

	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm
4 mm	135.414	135.415	135.416	135.417	135.418
6 mm	135.419	135.420	135.421	135.422	135.423



Conventional

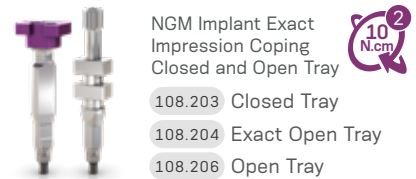

NGM Exact Titanium Base for Crown Ø 3.5

	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm
4 mm	135.414	135.415	135.416	135.417	135.418
6 mm	135.419	135.420	135.421	135.422	135.423




GM Titanium Base Burn-out Coping

4 mm	118.322	118.323	Ø 3.5
------	---------	---------	-------

Drivers



Accessories



*Application of a film carbon-based coat that provides a lower friction coefficient, resulting in increased pre-load.

NGM Temporary Abutment



Single-unit screw-retained temporary prosthesis



Ø 3.5

Implant level.

Channels of customizations;


Retention portion height: 10 mm customizable up to 4 mm;

Exact.

Neo Removable screw;




Installation Sequence

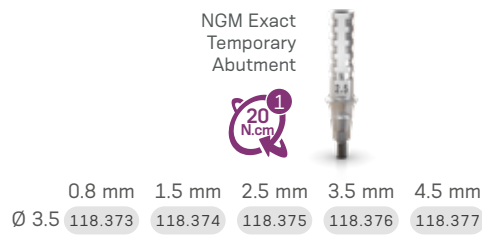

Customization

Temporary Prosthesis

Drivers



Neo Screwdriver Torque Connection

+



Torque Wrench

Accessories



Replacement Sterile Screws

116.294 Titanium


116.293 Neotorque*

*Application of a film carbon-based coat that provides a lower friction coefficient, resulting in increased pre-load.


NGM Attachment TIN



Overdenture

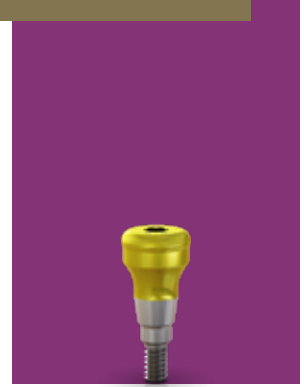


Installation Sequence

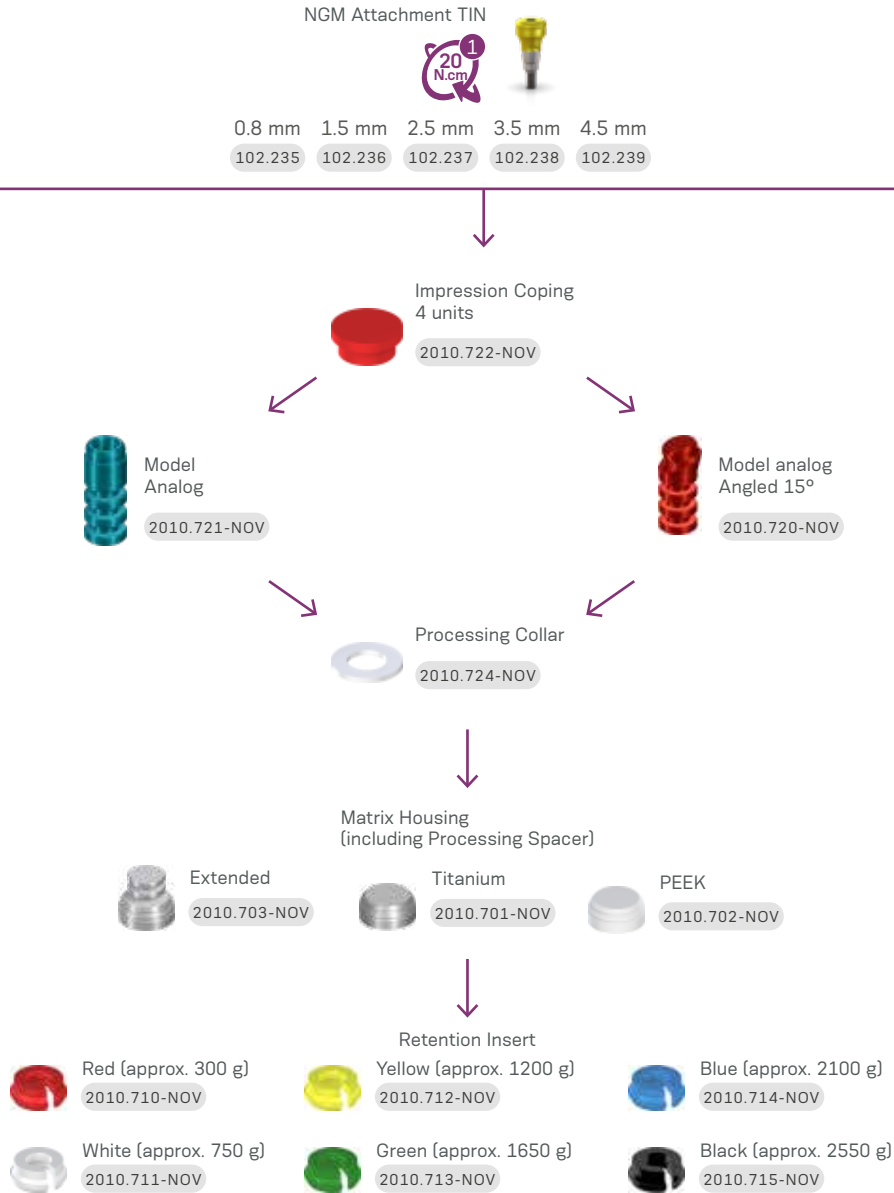

116

Drivers



Accessories





GM Narrow Kit

GM Narrow Surgical Kit

Autoclavable polymer case.

To order the pre-mounted version of the kit, with its complete composition, use code [110.316](#).



Articles

[110.315](#) Helix NGM Compact Surgical Kit Case

[103.585](#) NGM Guided Surgery Mucosa Punch

[103.586](#) NGM Initial Drill

[103.587](#) NGM Guided Surgery Bone Levelling Drill

[103.588](#) NGM Guided Surgery Initial Drill

[103.589](#) NGM Drill 2.0x10 mm

[103.590](#) NGM Drill 2.0x12 mm

[103.591](#) NGM Drill 2.0x14 mm

[103.592](#) NGM Drill 2.9x10 mm

[103.593](#) NGM Drill 2.9x12 mm

[103.594](#) NGM Drill 2.9x14 mm

[103.595](#) NGM Countersink Drill

[104.050](#) Torque Wrench

[104.060](#) Neo Manual Screwdriver (Medium)

[105.132](#) Neo Screwdriver Torque Connection

[105.137](#) Hexagonal Prosthetic Driver

[105.165](#) NGM Implant Driver For Contra-angle

[105.166](#) NGM Implant Driver For Torque Wrench

[128.036](#) NGM Height Measurer

[129.035](#) Helix NGM X-ray Positioner

Note: Items that compose Neodent® Kits are sold separately.

GM Narrow Instruments



NGM Guided Surgery Mucosa Punch

103.585



NGM Guided Surgery Bone Levelling Drill

103.587



NGM Guided Surgery Initial Drill

103.588



NGM Initial Drill

103.586



NGM Tapered Drills

- 103.589 Ø2.0 x 10mm
- 103.590 Ø2.0 x 12mm
- 103.591 Ø2.0 x 14mm
- 103.592 Ø2.9 x 10mm
- 103.593 Ø2.9 x 12mm
- 103.594 Ø2.9 x 14mm



NGM Countersink Drill

103.595



NGM Implant Driver - Contra Angle

105.165



NGM Implant Driver - Torque Wrench

105.166



NGM Height Mesurer

128.036



Helix NGM X-ray Positioner

129.035



Neo Manual Screwdriver

- :: Available in surgical steel;
- :: Yellow color for line identification

Medium
25 mm

104.060



Neo Screwdriver Torque Connection - Torque Wrench

- :: Available in surgical steel;
- :: Yellow color for line identification.

Medium
22 mm

105.132



Hexagonal Prosthetic Driver

- :: Available in surgical steel;
- :: To install and apply torque over straight GM Mini Conical Abutments and GM Micro Abutments;
- :: Yellow color for line identification.

Torque Wrench

105.137



Torque Wrench

- :: Available in surgical steel;
- :: Fitting for square connections;
- :: Collapsible Wrench that allows for proper assembly cleaning.

104.050



Sleeve D2.93


- :: Available in titanium;
- :: Sold in bags with 10 units each.

125.180

Neodent[®] Techniques

One Step Hybrid Technique

The One Step Hybrid technique allows the passive fitting of prosthesis, without the need for weld procedure, by cementing the neo micro/mini titanium abutment coping base into the metal structure. This technique allows as well through a digital workflow, milled dental structure to be cemented on top of this titanium abutment coping. It is indicated for multi-unit screw-retained prosthesis and results in reduced laboratory work times. It can be performed over GM Mini Conical Abutments or GM Micro Abutments. The sequence to perform the One Step Hybrid technique is described in the following pictures:

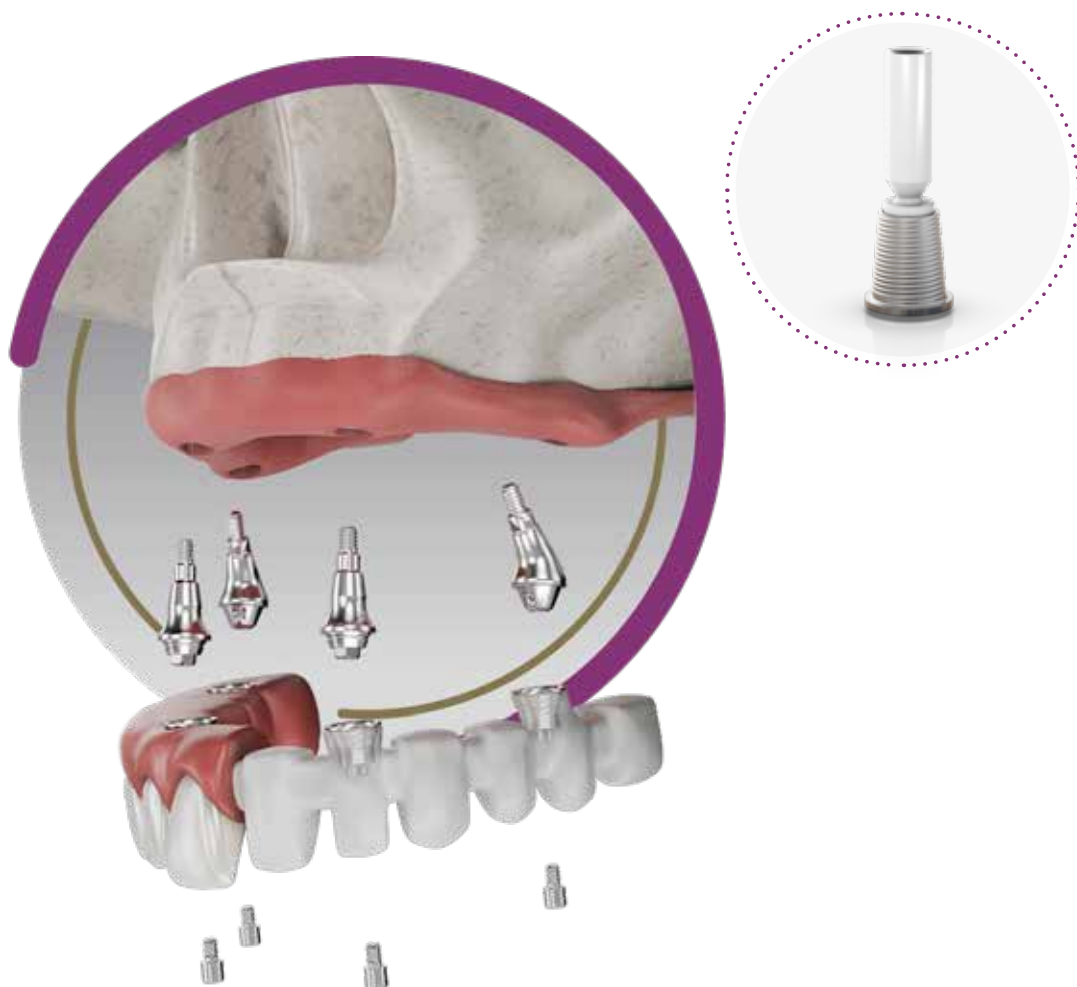

Neo Mini Conical Abutments Copings One Step Hybrid Technique

:: For installation, use the Neo Torque Connection (105.132);
 :: For torque control, use Torque Wrench (104.050).

Burn-out	Brass	Titanium
118.340	118.331	118.382



Neo Micro Conical Abutments Copings One Step Hybrid Technique

:: For installation, use the Neo Torque Connection (105.132);
 :: For torque control, use Torque Wrench (104.050).

Burn-out	Brass	Titanium
118.341	118.333	118.381



Neo Working Screw One Step Hybrid

:: For laboratory use.

116.271


Demonstration Sequence



Regularize the alveolar ridge.



Surgical drilling completed, obtaining adequate distance from distal implant in relation to the mental foramen with 7 mm Space Planning Instrument.

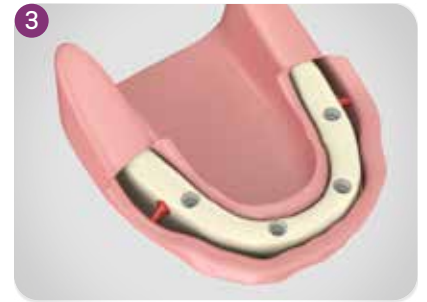

Placement of 4 Neodent® implants, according to their indication.



Placement of corresponding Neodent® Abutments.



Placement of Impression Copings, splinted with acrylic resin.



Positioning of Multifunctional Guide to obtain intermaxillary correlation. Soft silicone is injected to take the soft tissue impression.




Removal of Multi-Functional Guide and placement of Analog to the impression copings.



Working model with artificial gum.

Option 1 -Conventional Workflow for cast framework

Neo Mini Abutments Copings One Step Hybrid Technique

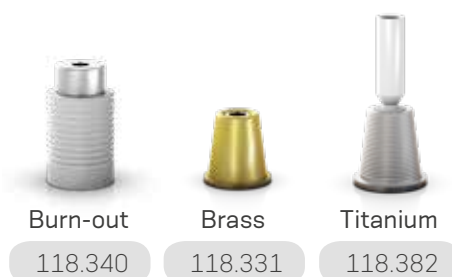

1 Working model with artificial gum.



2 Brass Copings are placed over analogs, then Burn-out Copings are fixed by working screws.




3 Wax-up the framework.



4 Cast framework. If necessary, provide internal wear in the regions corresponding to the castable copings.



5 Placement of both the Neo Mini Conical Abutment Coping Base and the sealing pin on top of the analog.

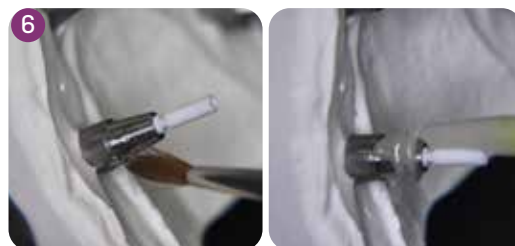

6 Apply a specific primer and proceed with the cementation according to the cement manufacturer.



7 Press the infrastructure over the coping base and immediately remove any overflowed cement excess as well as the sealing pin.



8 Unscrew the infrastructure from the model. Final framework with ensured passivity.

Option 2- Digital Workflow for milled Zirconia Bar

Neo Mini Conical Abutment Coping Base



Titanium

118.382



Working model with artificial gum.



Install the GM Mini Conical Abutment Scanbody on the model and proceed with the scanning.



Design the zirconia bar in the CAD/CAM software.



Mill the zirconia bar.



Placement of both the Neo Mini Conical Abutment Coping Base and the sealing pin on top of the analog.



Apply a specific primer and proceed with the cementation according to the cement manufacturer.



Press the infrastructure over the coping base and immediately remove any overflowed cement excess as well as the sealing pin.



Unscrew the infrastructure from the model. Final framework with ensured passivity.



Final framework.

Distal Bar Technique

Technique used to ease mandible rehabilitation, through a provisional hybrid type prostheses supported by implants.



Neo Distal Bar Coping

- :: Available in titanium;
- :: Retainers to ease joining with acrylic resin;
- :: Recommended torque: 10 N.cm;
- :: For torque, use Neo Screwdriver (105.132)

118.308



Neo Distal Bar

- :: Recommended for distal Implants to reinforce the cantilever.

125.116



Polishing Protector

- :: Available in surgical steel;
- :: Protection for the lab polishing.

123.008

Demonstration Sequence



1 Neodent® Abutments placed.




2 Prosthesis wearing, keeping posterior region integrity.




3 Place the copings into the central Implants and Distal Bar to distal Implants.




4 Proof of inferior prostheses wearing (centered occlusion position, no interference on copings).

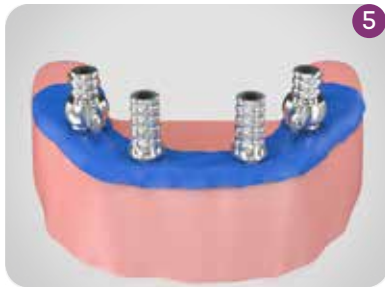

5 Placement of rubber dam over copings to protect soft tissues.

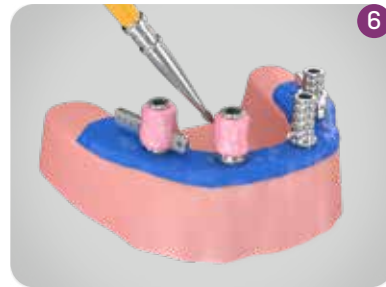

6 Apply selfpolymerizing acrylic resin on and between the copings.

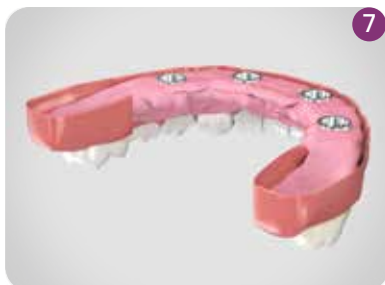

7 Apply to worn area in lower prosthesis, repositioning inside mouth. Keep patient in occlusion until total polymerization.



8 Remove the inferior prosthesis after resin is polymerized. Copings already captured.



9 Adjustments, finishing and polishing procedures of inferior prosthesis with polishing protectors.



10 Placed provisional implant supported prosthesis.



11 Final inside-mouth posterior view.

Digital Solutions



Visit www.neodent.com/cadcam to download the digital files to work with Neodent® Titanium Bases, Titanium Blocks, Abutments, Mini Conical Abutments, Micro Abutments, Universal Abutments, One Step Hybrid Copings, Scanbodies and Hybrid Repositionable Analogs. Libraries are available for the following companies: exocad GmbH, Amann Girrbach AG Inc, Dental Wings Inc and 3Shape A/S.

Scanbody

Neodent® Scanbodies can be used for scanning and digitalization of the patient or model providing accuracy in determining the analog position.



- 108.207 GM Exact Implant Intraoral Scanbody
- 108.218 GM Mini Conical Abutment Scanbody (intraoral and model)
- 108.219 GM Micro Abutment (intraoral and model)
- 108.220 GM Abutment (intraoral and model)
- 108.222 Zi Implant Scanbody
- 108.221 NGM Implant Scanbody



Compatible with
Neo Screwdriver

Hybrid Repositionable Analog

Neodent® Hybrid Repositionable Analogs can be used in prototyped models, produced by 3D printers, or conventional plaster models.



- 101.103 GM Hybrid Repositionable Analog 3.5/3.75
- 101.089 GM Hybrid Repositionable Analog 4.0/4.3
- 101.090 GM Hybrid Repositionable Analog 5.0/6.0
- 101.091 Micro Abutment Hybrid Repositionable Analog
- 101.092 Mini Conical Abutment Hybrid Repositionable Analog
- 101.097 Universal Abutment Hybrid Repositionable Analog 3.3X4
- 101.098 Universal Abutment Hybrid Repositionable Analog 3.3X6
- 101.099 Universal Abutment Hybrid Repositionable Analog 4.5X4
- 101.100 Universal Abutment Hybrid Repositionable Analog 4.5X6
- 101.101 GM Abutment Hybrid Repositionable Analog

General Instruments

Torque Wrench

- :: Available in surgical steel;
- :: Extremely safe (lower than 5% variation);
- :: Fitting for square connections;
- :: Collapsible Wrench that allows for proper assembly cleaning.

104.050



Operational Instructions

The Neodent® Torque Wrench was designed to allow the necessary torque to be applied and simultaneous verification of that torque with the same Instrument.



All that is needed is to apply force to the wrench handle **1** (never the wrench body) until the value marked on the LATERAL SCALE **2** corresponds to the desired torque.

The wrench function works in both directions, by simply pulling and turning the driver's pin 180°. However, the torque measurements work only lockwise.



•WARNING: When inverting the torque direction, the gear may come loose from the driver body and fall. Therefore, this inversion should only be done with the driver connected to a part or outside the patient's mouth.



The Neodent® Torque Wrench comes with pre-calibrated torques

Titanium Tweezers

- :: To handle implants;
- :: New Tweezer system that prevents deviation in the active bit;
- :: Millimeter scale for checking during procedures;
- :: Self-locking implant.

129.001



Depth Probe

- :: Available in titanium;
- :: To probe preparations and analyze depth;
- :: Millimeter scale for checking during procedures.

129.004



7 and 9 mm Space Planning Instrument

- :: Available in surgical steel;
- :: Recommended for prosthetic/surgical planning;
- :: 7 and 9 mm marks.

128.026



Surgical Labial Retractor

- :: Available in surgical steel;
- :: Rounded edges to minimize surgical trauma.

124.001



Columbia Retractor

- :: Available in surgical steel;
- :: Rounded edges to minimize surgical trauma.

124.003



Scapel Handle

- :: Available in surgical steel;
- :: For standard scalpel blade use;
- :: Blade not included.

129.008




Bivers Handle

- :: Available in surgical steel;
- :: Non-traumatic extraction for implant placement;
- :: Similar to a periosteal.

129.002




Concave Osteotome



:: Available in surgical steel;
 :: Concave active cutting bit for nontraumatic lifting the floor of the maxillary sinus;
 :: Used to prepare the surgical alveolus for Implant placement in the posterior maxillary region with low bone height;
 :: Marks from 7 to 17mm.
 :: Marks from 7 to 17mm.

- 1.8 mm 110.325
- 2.0 mm 110.323
- 2.5 mm 110.326
- 3.0 mm 110.327
- 3.5 mm 110.328
- 4.0 mm 110.329
- 4.5 mm 110.330

Convex Osteotome



:: Available in surgical steel;
 :: Convex active bit;
 :: Used when the bone width is insufficient, demanding bone compression and expansion before placing the implant;
 :: Marks from 7 to 17mm.

- 1.8 mm 110.331
- 2.5 mm 110.332
- 2.9 mm 110.324
- 3.0 mm 110.333
- 3.5 mm 110.334

Osteotomes Kit Case

:: Available in polymer;
 :: Autoclavable;
 :: Osteotomes sold separately.



110.262


Surgical Hammer



:: Available in surgical steel;
 :: Polymer active bit;
 :: Used in compactors and expanders;
 :: Weight: 130g.

126.001

Trephine Bur



:: Available in surgical steel;
 :: Collecting bone cylinder;
 :: Implant removal.

- Ø 3.3 103.051
- Ø 3.5 103.490
- Ø 3.75 103.491
- Ø 4.1 103.026
- Ø 4.3 103.087
- Ø 5.0 103.027
- Ø 8.0 103.028

Sinus Lift Curette

:: Available in surgical steel;
 :: Used to displace the Sinusal Membrane.



- 1 126.008
- 3 126.009
- 4 126.010
- 5 126.011
- 7 126.012

Complement Case



:: Available in autoclavable polymer;
 :: Used to organize drills and auxilliary connections.

110.270

Handle Implant Driver



:: Available in stainless steel;
 :: Manual implant placement.

104.047

Analog Handle



:: Used for tightening analogs and milling prosthetic abutments.

104.036

Prosthetic Surgical Guide



:: Available in titanium;
 :: Abutments to prepare the surgical guide;
 :: Prosthetic guide inner diameter 2 mm
 :: Heights 6 and 10 mm;
 :: Surgical Guide: package with 10 units (5 units of 10 mm and 5 units of 6 mm);
 :: Surgical Guide Pin: package with 5 units

- Guide 103.092
- Pin 103.093



Neodent[®] *global play* >

Neodent[®] Global Play is an amazing **Training and Education online platform** that gathers great content available **on-demand for free**. You will find **clinical cases, product training videos, tutorials, and experts from around the world giving testimonials about Neodent[®] products**. In addition to that, you will have access to the **support material library** for instant download and updated with the latest **Neodent[®] events**, such as Neodent[®] Global e-Symposium and Zi Virtual Launch.

Registration is simple and automatic: fill out the form to have instant access to all the great content.



CHECK AT
globalplay.neodent.com





The Neodent® Congress reaches its 6th edition, in the same year that the Neodent® celebrates 30 years of existence.

May 18th, 19th and 20th, 2023.

Celebrate the Evolution

of implant dentistry, technology, the market, aesthetics, patients, and Neodent®!



Advanced periodontology applied to oral implantology



Ceramic implants: a new mindset



Digital dentistry in daily practice



Immediate Loading: breaking paradigms



Interdisciplinary and modern planning of the smile



Prosthetic principles leading to immediate loading success




Success Journey in Immediate Loading



Learn everything about the event!
Scan the QR Code or go to:
neodentcongress.com.br/en



 NEODENT

30 years



References

- [1] Novellino MM, Sesma N, Zanardi PR, Laganá DC. Resonance frequency analysis of dental implants placed at the posterior maxilla varying the surface treatment only: A randomized clinical trial. *Clin Implant Dent Relat Res*. 2017 Jun 20. doi: 10.1111/cid.12510. [Epub ahead of print]
- [2] Sartoretto SC, Alves AT, Resende RF, et al. Early osseointegration driven by the surface chemistry and wettability of dental implants. *J Appl Oral Sci*. 2015 May-Jun;23(3):279-87.
- [3] Sartoretto SC, Alves AT, Zarranz L, et al. Hydrophilic surface of Ti6Al4V-ELI alloy improves the early bone apposition of sheep tibia. *Clin Oral Implants Res*. 2016 Jun 17. doi: 10.1111/clr.12894. [Epub ahead of print]
- [4] Val JE, Gómez-Moreno G, Ruiz-Linares M, et al. Effects of Surface Treatment Modification and Implant Design in Implants Placed Crestal and Subcrestally Applying Delayed Loading Protocol. *J Craniofac Surg*. 2017 Mar;28(2):552-558.
- [5] Al-Nsour MM, Chan HL, Wang HL. Effect of the platform- switching technique on preservation of peri-implant marginal bone: a systematic review. *Int J Oral Maxillofac Implants*. 2012 Jan-Feb;27(1):138-45.
- [6] Annibali S, Bignozzi I, Cristalli MP, et al. Peri-implant marginal bone level: a systematic review and meta-analysis of studies comparing platform switching versus conventionally restored implants. *J Clin Periodontol*. 2012 Nov;39(11):1097-113.
- [7] Hsu YT, Lin GH, Wang HL. Effects of Platform-Switching on Peri-implant Soft and Hard Tissue Outcomes: A Systematic Review and Meta-analysis. *Int J Oral Maxillofac Implants*. 2017;32(1):e9-e24.
- [8] Lazzara RJ, Porter SS. Platform switching: a new concept in implant dentistry for controlling postrestorative crestal bone levels. *Int J Periodontics Restorative Dentistry*. 2006 Feb;26(1):9-17.
- [9] Rocha S, Wagner W, Wiltfang J, Nicolau P, Moergel M, Messias A, Behrens E, Guerra F. Effect of platform switching on crestal bone levels around implants in the posterior mandible: 3 years results from a multicentre randomized clinical trial. *J Clin Periodontol*. 2016 Apr;43(4):374-82.
- [10] Babbush CA. Post treatment quantification of patient experiences with full-arch implant treatment using a modification of the OHIP-14 questionnaire. *J Oral Implantol*. 2012 Jun;38(3):251-60.
- [11] Block MS, Haggerty CJ, Fisher GR. Nongrafting implant options for restoration of the edentulous maxilla. *J Oral Maxillofac Surg* 2009;67:872–881.
- [12] Steigenga J, Al-Shammari K, Misch C, Nociti FH Jr, Wang HL. Effects of implant thread geometry on percentage of osseointegration and resistance to reverse torque in the tibia of rabbits. *J Periodontol*. 2004;75(9):1233-41.
- [13] Carvajal Mejía JB, Wakabayashi K, Nakano T, Yatani H. Marginal Bone Loss Around Dental Implants Inserted with Static Computer Assistance in Healed Sites: A Systematic Review and Metaanalysis. *Int J Oral Maxillofac Implants*. 2016 Jul-Aug;31(4):761-75.1.
- [14] Pozzi A, Tallarico M, Marchetti M, Scarfò B, Esposito M. Computer-guided versus free-hand placement of immediately loaded dental implants: 1-year post-loading results of a multicentre randomized controlled trial. *Eur J Oral Implantol*. 2014 Autumn;7(3):229-42.
- [15] Hultin M, Svensson KG, Trulsson M. Clinical advantages of computer-guided implant placement: a systematic review. *Clin Oral Implants Res*. 2012 Oct;23 Suppl 6:124-35.
- [16] Soares MM, Harari ND, Cardoso ES, et al. An in vitro model to evaluate the accuracy of guided surgery systems. *Int J Oral Maxillofac Implants*. 2012 Jul-Aug;27(4):824-31.
- [17] Pozzi A, Polizzi G, Moy PK. Guided surgery with tooth-supported templates for single missing teeth: a critical review. *Eur J Oral Implantol*. 2016;9(1)135-53.

Neodent®, Zi®, ZiLock®, NeoPoros, Acqua, Helix®, Drive®, Titamax®, Grand Morse®, Helix GM®, Drive GM®, Titamax GM®, Neotorque, NeoArch®, Zygoma GM™ are trademarks or registered trademarks of JIGC Indústria e Comércio de Materiais Dentários S.A.

CEREC is a trademark or registered trademark of Sirona Dental Systems GmbH (DE).

Dentsply Sirona is a trademark or registered trademark of Dentsply Sirona, Inc.

MEDENTIKA is a trademark or registered trademark of Medentika GmbH.

Novaloc is a trademark or registered trademark of Valoc AG.

Panavia is a trademark or registered trademark of Kuraray Co. Ltd.

Amann Girrbach is a trademark or registered trademark of Amann Girrbach AG.

exocad is a trademark or registered trademark of exocad GmbH.

Dental Wings is a trademark or registered trademark of Dental Wings Inc.

3Shape is a trademark or registered trademark of 3Shape A/S.

